


Operation Manual

Polytector III G999

1 to 7 gas warning device with electrical suction pump

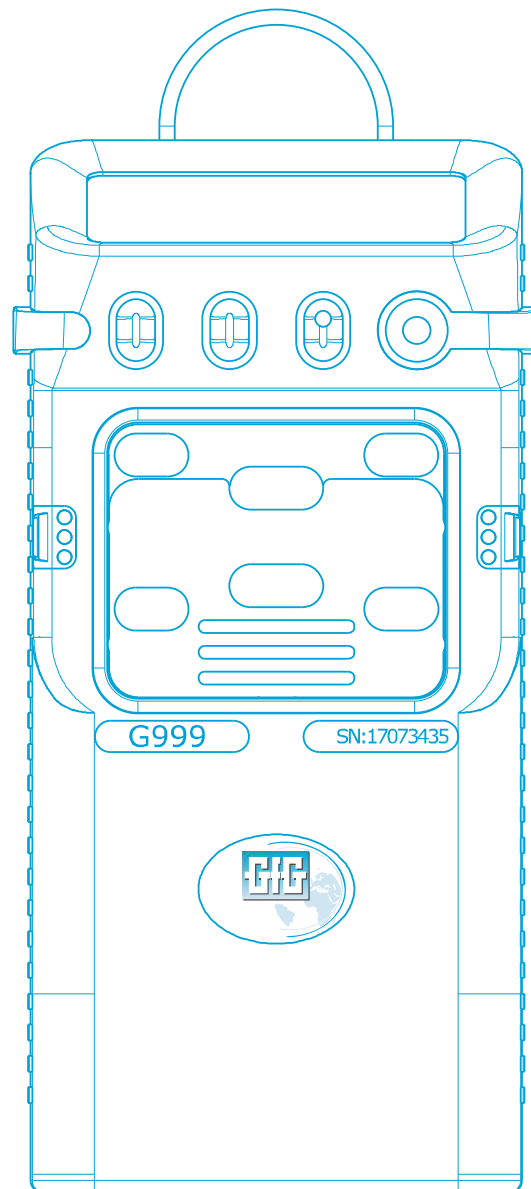

Measurable safety by using GfG devices

Congratulations!

You have chosen a precision instrument made by GfG.
A very good choice!

Since reliability, safety, optimum performance and efficiency distinguish our devices.

They comply with the national and international directives.

These operating instructions will help you to rapidly and safely operate the device.

Please strictly follow our operating instructions before commissioning!

Our employees will be at your service at any time in case of inquiries.

Yours

GfG Gesellschaft für Gerätebau mbH

Klönnestraße 99

D-44143 Dortmund

Phone: +49(0)231 – 564 00-0

Fax: +49(0)231 – 51 63 13

E-mail: info@gfg-mbh.com

Internet: www.gasmessung.de


Table of contents

	Page
1 INTRODUCTION	5
1.1 For your safety	5
1.2 Area of use and application	5
1.3 Special conditions for the safe use	5
1.4 Design	6
2 OPERATING INSTRUCTIONS	6
2.1 Commissioning	6
2.1.1 Switching the device on and off	6
2.1.2 Other messages when starting the device	7
2.2 Measuring mode	8
2.2.1 Battery capacity and battery alarm	8
2.2.2 Gas alarm signalling	8
2.2.3 Acknowledging the gas alarms	9
2.2.4 Short term, long term, maximum, minimum values	9
2.2.5 Zoom display and turning the display	9
2.2.6 Peak display of the peak values	9
2.2.7 Operation with an integrated suction pump	9
2.2.7.1 Switching the pump on and off	10
2.2.7.2 Status signal of the pump and Flow monitoring	10
2.2.7.3 Minimum pumping time	10
2.2.8 Use of the flash light	10
2.2.9 Display lighting	10
2.2.10 Recording of measurement data with the data logger	11
2.2.11 Influence of oxygen and interference gases	11
2.2.12 Peculiarities when monitoring in the LEL range	11
2.2.13 HI% measurement of methane or natural gas	11
2.3 Service mode	12
2.3.1 Main menu	12
2.3.1.1 Place – Choice of a measuring point	12
2.3.1.2 Name – Choice of a device user	12
2.3.1.3 AutoCal – Menu for AutoCal adjustment	12
2.3.1.4 Sensor overview	13
2.3.1.5 System information	13
2.3.2 Service menu	13
2.3.2.1 System menu for system settings	14
2.3.2.1.1 Bump test	14
2.3.2.1.2 Sensor adjustment (zero point + calibration)	14
2.3.2.1.3 Inspection	15
2.3.2.1.4 Time	15
2.3.2.1.5 System options	15
2.3.2.1.6 Sensor choice – Activation / deactivation of sensors	16
2.3.2.1.7 AutoCal air – Sensor release for AutoCal adjustment	16
2.3.2.1.8 AutoCal gas – Sensor release for AutoCal adjustment	16
2.3.2.2 Sensor menu for sensor settings	16
2.3.2.2.1 Zero – Adjusting the zero point	17
2.3.2.2.2 Calibrating – Sensitivity adjustment	17
2.3.2.2.3 Alarms – Alarm setting	18
2.3.2.2.4 Calibration data	18
2.3.2.2.5 Information	18
2.3.2.2.6 Measuring range	19
2.3.2.3 Data logger settings	19
2.4 Power supply	20
2.4.1 Charging the battery	20
2.4.2 Lazy battery effect on the NiMH battery and its removal	21
2.4.3 Changing the battery module	21
3 ANNEX	21
3.1 Maintenance	21
3.2 Maintenance and inspection	21
3.3 Maintenance - Repair	22
3.4 Calibration device	22
3.5 Inspection with the docking station DS400	22
3.6 Malfunction, cause, remedy	23
3.7 Accessories and spare parts	24
3.8 Indications regarding the environmentally friendly disposal	24

3.9	Sensor types and measuring ranges	25
3.10	Sensor specification	26
3.11	Alarm limit values - Basic setting	31
3.12	Technical data	32
3.13	EU-Type Examination Certificate	33
3.14	EU-Declaration of Conformity	34

1 Introduction

1.1 For your safety

These operating instructions point to the intended use of the product and serve to avoid dangers according to § 3 of the Product Safety Act. It must be read and observed by everyone who operates, services, maintains and inspects this product. This is particularly relevant for the safety instructions in this manual marked with this symbol . This device can serve its intended purpose only if it is operated, serviced, maintained and inspected according to the instructions given by the Gesellschaft für Gerätebau mbH. The warranty assumed by the company GfG Gesellschaft für Gerätebau mbH forfeits, if it is not used, cared for, maintained and controlled according to the specifications of the company GfG.

The above mentioned does not change the indications about the warranty and liability in the sales and delivery conditions of the company GfG. Any repair works may only be performed by professionals or assigned employees. Any conversions and modifications on the product may only be performed with the approval of the GfG. Any unauthorised changes on the product exclude a liability for damages. Only use accessories made by the GfG together with the product. Use the spare parts released by the GfG for any repairs.

A functional test **has to** be performed on every working day before each use - a calibration and, if applicable, an adjustment needs to be performed every 4 months.

1.2 Area of use and application

The G999 is a hand-held meter which serves for the personal protection against dangers caused by toxic or explosive gases and vapours as well as by lack of or excess oxygen. The G999 permanently measures in the diffusion mode or by sucking the gas with the integrated pump and warns the employee carrying the device in case of an occurring gas hazard by a visual and acoustical alarm.

The three variants of the G999 have been tested by the DEKRA EXAM GmbH concerning the use in potentially explosive atmospheres and possesses a corresponding EU type examination certificate according to the directive 2014/34/EU as well as an IECEx certificate.

Certificates: **BVS 15 ATEX E 064 X**
IECEx BVS 15.0056 X

Labelling: **G999C**  I M2 Ex ia db I Mb  II 2G Ex ia db IIC T4 Gb -20°C≤Ta≤+50°C
G999E  I M1 Ex ia I Ma  II 1G Ex ia IIC T4 Ga -20°C≤Ta≤+50°C
G999P  I M1 Ex ia I Ma  II 1G Ex ia IIC T4 Ga -20°C≤Ta≤+50°C

1.3 Special conditions for the safe use



Caution: For use in hazardous areas of Group I (mining), the G999C must be used as intended. The device must be worn at the body and must not be left unattended so that mechanical stress due to impact is avoided. It is intended for low level mechanical hazards according to EN 60079-0.


The gas meter must be removed from the hazardous area and has to be cleaned immediately, if it is contaminated with oils and greases or hydraulic fluid.

Before each use, it is necessary to check the gas readings of flammable gases and vapours for zero gas and for test gas. If the gas readings show a continuous zero offset in an environment exempted from measuring gas, a zero point adjustment needs to be performed.

In particular after a heavy impact, the zero points of the sensors need to be controlled and readjusted, if required. If the catalytic combustion sensor would cause that the measuring range has been exceeded " " due to an impact stress, this alarm needs to be acknowledged with fresh air and, if applicable, the zero point needs to be readjusted.

If the G999 is being operated without interruption for more than one day, it should be switched off and on latest after 24 hours.

1.4 Design

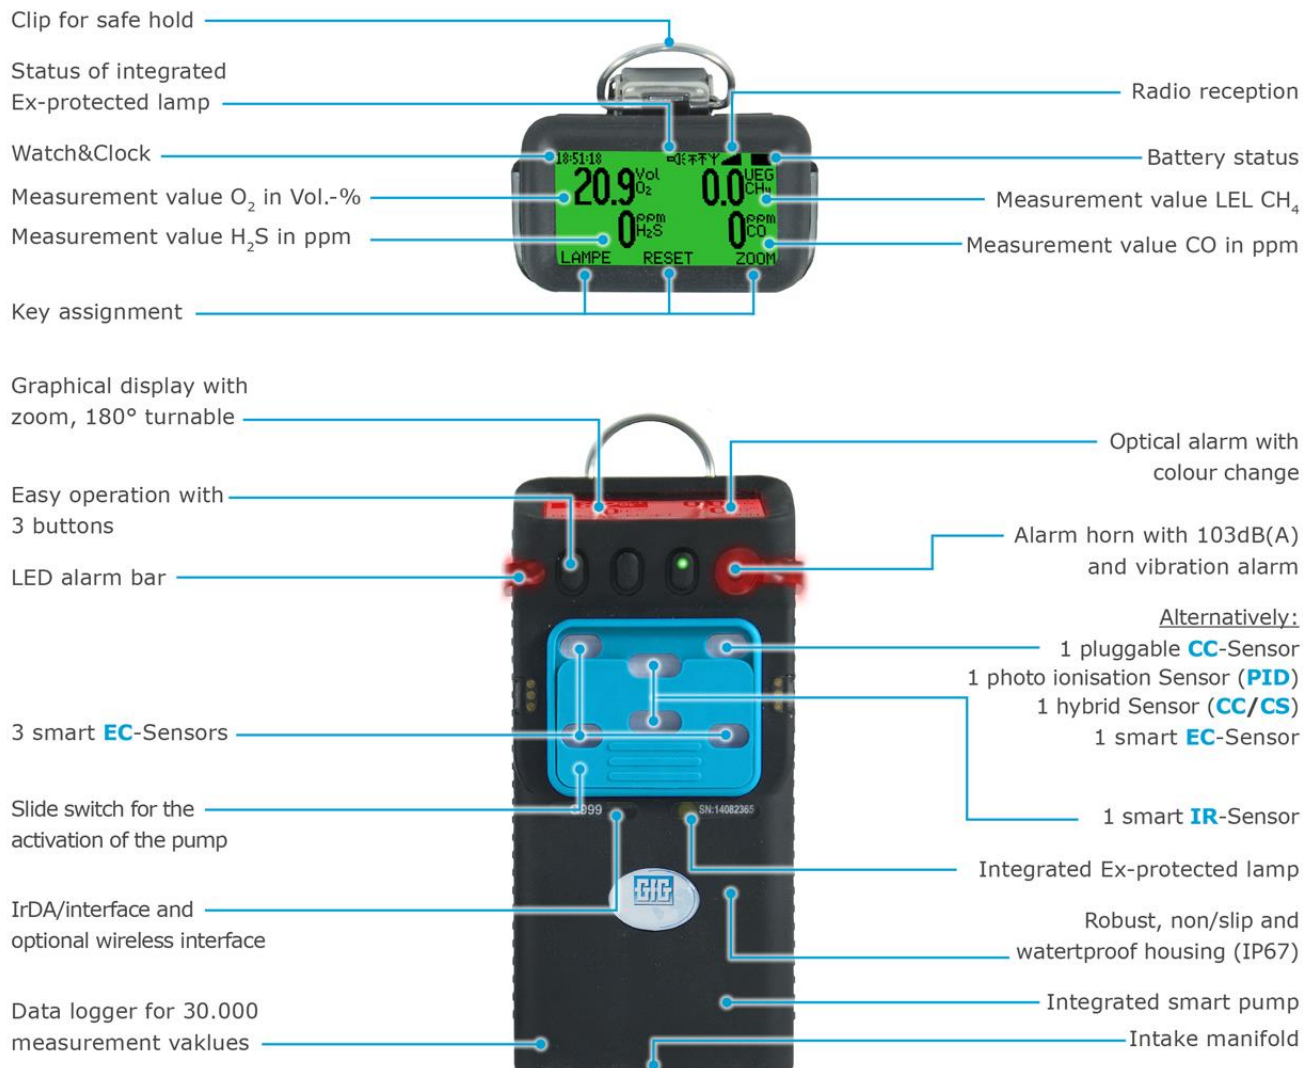



2 Operating Instructions

2.1 Commissioning

2.1.1 Switching the device on and off




Switch on the device by briefly pressing the right button .

Switch off the device by pressing the right button  for about 5 seconds. Release the button when the display "Switch off / 0" is shown.

When charging the device, the normal measuring mode is automatically switched off and the charging time will be displayed.

After having switched off the device, it performs a **self-test** and gives information about the Firmware version, the built-in sensors with their measuring ranges and the alarm thresholds as well as the date of the next inspection. During the self-test, the visual and acoustical signal transmitters will be controlled in a way that the user would recognise a gas alarm.

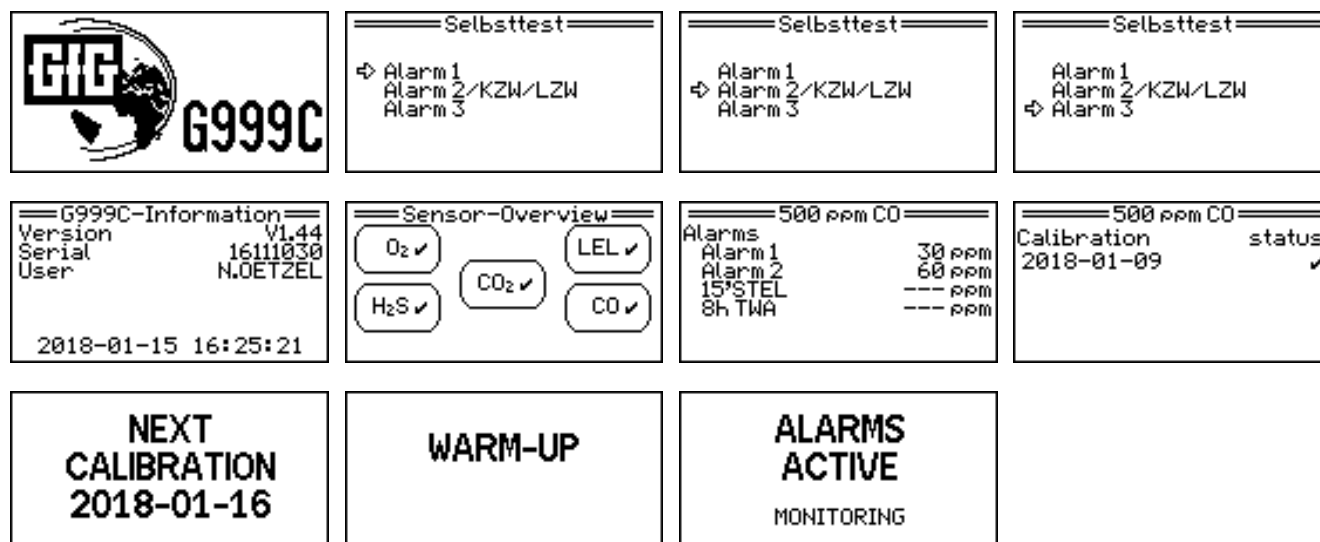


Alarm thresholds and calibration data will be displayed for all available sensors. Please find an example of CO below. Depending on the condition of the sensors, other messages will be output, which possibly need to be acknowledged. Please find more detailed information in the chapter "Other messages when starting the device".


After having switched on the device and the passing of the messages, the device will be ready for operation after about one minute. By pressing the centre button, it is possible to acknowledge displays and messages.

2.1.2 Other messages when starting the device


The G999 will test the sensors when starting the device and monitors the adjustment data. For a sensor, which had not been adjusted yet or which had been adjusted more than one year ago, the message "Sensor adjustment required!" will be the output. Since almost used up sensors might have a reduced adjustment interval in which case the message "Sensor adjustment or sensor replacement required!" will be the output. In case of used up sensors, the message "Sensor replacement required!" will be the output when the device would be started. These messages need to be acknowledged by pressing the button.

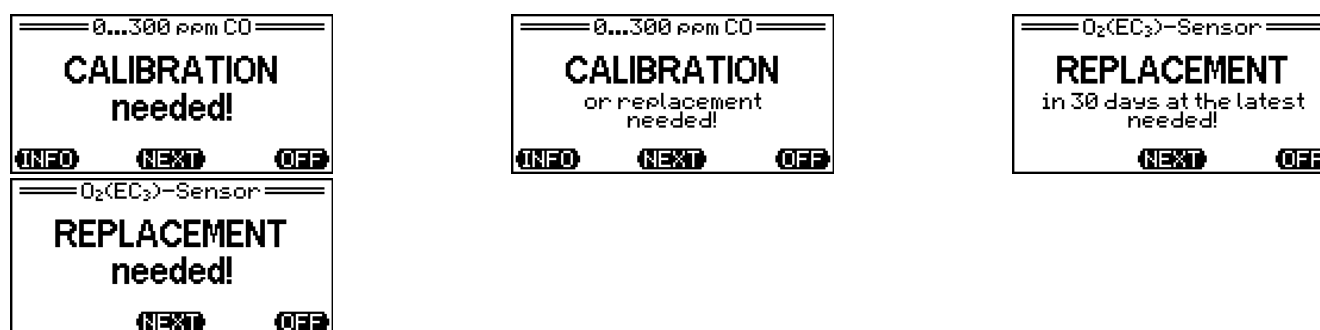

If a docking station is used to check the device, then the intervals for the functional test and for the sensor adjustment might have been set in the G999. The dates for the next functional test or the next sensor adjustment automatically result of the time of the last tests. Depending on what will be due next, the date of the next functional test or of the next sensor adjustment will be displayed when starting the device. If a date has already been exceeded, the G999 will notify this "overdueness". These messages need to be acknowledged by pressing the button.

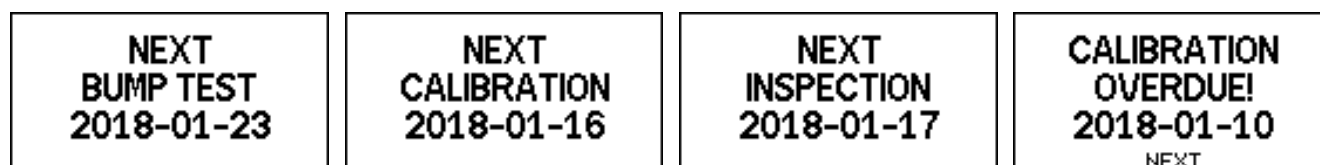

2.2 Measuring mode




The G999 is ready for operation, if all measured values, the measuring gas or the unit, the battery capacity and the time are displayed.

If more than five measured values are displayed simultaneously, the time will no longer be displayed due to lack of space.

The measured gas concentrations will now be monitored regarding exceeding or falling below (O_2) the preset limit values.

If more than two measured values are displayed simultaneously, either only the type of gas or only the unit will be displayed. By pressing the right button (**ZOOM**) the measured values are individually displayed with the number of units and the type of gas.

2.2.1 Battery capacity and battery alarm



In the measuring mode, the capacity of the battery can be read from the state of charge icon on the left of the display. The black filling represents the remaining capacity. By pressing the right button (**ZOOM**) it is also possible to display the remaining capacity as a figure. (*1)

Generally, the fully charged battery would have a capacity for a continuous operation of more than 8 hours (11...130 hours depending on the sensor combination - also refer to the technical data). The service life can be reduced by alarms. If the state of charge drops to such a low level that the state of charge icon is no longer filled out, the device will switch to the "Energy-saving mode". From this moment on, the green display lighting will no longer be activated when pressing a button. In case of a gas alarm, the red display lighting will also no longer be used. Then, the alarm signalling only occurs with the red alarm LEDs with a maximum horn volume of 90dB(A). If the state of charge drops even further, the battery alarm would be triggered and signalled acoustically. In this condition, the state of charge icon will flash. The maximum remaining service life is displayed in minutes. After 15 minutes, the device will automatically switch off with a clear acoustical signal. Then, the message "OFF" will be displayed for 5 minutes. If the function "Anti-Lazy-Battery" has been activated in the option menu, the device will not be automatically switched off after 15 minutes, but only when the minimum voltage falls below.

2.2.2 Gas alarm signalling

If the measured gas concentration exceeds a preset limit value, an acoustical and visual alarm will be immediately emitted. It is possible to read from the display which gas has triggered the alarm. An extremely loud acoustical alarm (103 dB(A) at 30 cm) and a bright visual all-round alarm provide for a safe warning in case of a gas hazard. In case of a gas alarm, the whole display will be coloured orange or red, depending on the alarm condition. The device has up to three alarm levels. The pre-alarm AL1 is not self-holding, whereas the main alarms AL2 and AL3 are self-holding (factory setting). The G999 makes three limit value alarms available for oxygen and flammable gases (e.g. CH_4) and it makes two limit value alarms available for toxic gases (e.g. CO , H_2S). An alarm can additionally be emitted for the toxic gases if the long-term and the short term limit value (LZW and KZW) have been exceeded. Also refer to the chapters "Alarm limit value - Basic setting" and "Alarms - Alarm setting". The alarm signalling can additionally be emitted by vibrations, if a corresponding "supply module with vibrator" is built in.


Type of alarm	Sensors	Number of alarms	Description
Limit value (AL)	Oxygen	3	A limit value alarm is immediately being triggered, if the gas concentration exceeds or falls below a preset value (O_2). The limit value alarms can be set.
	Flammable gases	3	
	Toxic gases	2	
Short-term value (KZW)	Toxic gases	1	The short-term value (KZW) refers to a period of time of 15 minutes and the mean will be taken over this period of time. The short-term value (KZW) alarm is not self-holding. It will automatically switch off as soon as the short-term limit value falls below once again.
Long-term value (LZW)	Toxic gases	1	The long-term value (LZW) refers to a period of time of a working shift of 8 hours and the mean will be taken over this period of time. The LZW alarm cannot be reset. It will only be switched off if the device is being switched off.

The alarms will be prioritised as follows: Power error, exceeding the measuring range, AL3, LZW > AL2, KZW > AL1, falling below the measuring range > temperature error.

2.2.3 Acknowledging the gas alarms

The limit value alarms 2 and 3 are self-holding (factory setting) and can only be reset by pressing the button **RESET**, if it falls below or exceeds the preset limit values (O_2). The limit value alarm 1 is not self-holding and will be automatically reset as soon as the alarm condition does no longer exist.

If the measuring range is exceeded on the catalytic combustion sensor (e.g. CH_4), for gas concentrations above 110 % LEL or above 5.5Vol.% CH_4 arrows **↑↑↑** showing upwards will be displayed instead of the gas display. The sensor will be deactivated in order that it will not be damaged. The alarm signalling and the arrows **↑↑↑** showing upwards will be maintained. The alarm signalling can only be terminated by pressing the button **RESET**. Then, the following questions will be displayed:



Only if it is made sure that **there is no flammable gas on the sensor, but only fresh air, the question may be answered with YES**. In this case, the sensor will be reactivated and will display measured values after a short running-in period!

Please find further details in the chapter "Peculiarities when monitoring the LEL range".

2.2.4 Short term, long term, maximum, minimum values

After having switched on the device, it will continuously measure in the diffusion mode. All concentrations will be displayed in this operating mode. In addition, short term and long term values (KZW and LZW) will be formed for toxic gases and maximum and minimum values (MAX and MIN) will be saved for non-toxic gases.

These saved values can be displayed on the screen if the screen is switched over to the corresponding display mode by pressing the right mouse button **ZOOM**.

2.2.5 Zoom display and turning the display

The G999 allows turning the display on the screen by 180°. To do so, keep the left and right button pressed simultaneously and release it. In this way, the display can be easily read when the device is attached to the belt.

In order to be able to see the measured values on the **Zoom** display, press the **right button (ZOOM)**. Briefly press the button in order to zoom a displayed value. By pressing the right button several times, you can zoom the display of the measured values of the individual sensors one after another. When the display of a value is zoomed, you can long press the button **ZOOM** and change over to the following detailed view:




Example: Zoom display for H_2S

Top left: Maximum value
Top right: Current gas concentration
Bottom left: Short-term value (15 minutes)
Bottom right: Long-term value (8 hours)

Within one session you can change between the two zoom modes by long pressing the button **ZOOM**. After having activated a zoom display, the display generally skips to the normal view after about 10 seconds, depending on the configuration (system options). If the button **RESET** is pressed in the zoom display, the maximum value memory will be reset to the current gas concentration.

2.2.6 Peak display of the peak values



It is possible to monitor and display peak values in the peak mode which is activated by pressing the button **PEAK**. On the screen in the top row, the icon **↕↕** with the arrows is being displayed.

In the zoom display on the top left the corresponding peak value is displayed instead of the max. or min gas concentration.

If the button **RESET** is pressed in the peak mode, the peak memory will be reset to the current gas concentration. The peak mode will be deactivated by pressing the button **PEAK**.


2.2.7 Operation with an integrated suction pump

The integrated electrical suction pump can be used to suck in gases. If the G999 is switched to the operating mode, information and messages of the pump will be displayed on the screen of the G999 and malfunctions will be signalled visually and acoustically.

2.2.7.1 Switching the pump on and off

The pump will be switched on by pushing the sensor cover up. Then, the operating status of the pump will be displayed on the screen of the gas measurement device.



In case of a sufficient battery capacity the pump motor will switch on after a short delay of about 1 second. Then, the animated icon  for the pump is displayed in the top row.

The pump will be switched off by pushing the sensor cover down.





In doing so, the pump icon will fade out on the screen of the G999 gas measurement device.

In order that the batteries will not be discharged unnecessarily, the pump should be switched off after each measurement.

2.2.7.2 Status signal of the pump and Flow monitoring


During the pump operation, an additional pump icon which indicates the operating status of the pump will be displayed on the standard screen display of the G999 gas measurement device.




The undisrupted pump operation will be displayed at the top of the screen of the gas measurement device with a mobile pump icon .

This icon flashes if the pump is no longer fully functional.

Any other alarm and fault statuses will be acoustically and visually displayed on the alarm system of the G999 gas measurement device. In the normal pump operation, the supplied gas volume amounts to about 0.50...0.60slpm (slpm = standard litre per minute).



When the pump is switched on, the zoom mode of the display shows the currently aspirated distance of the suction hose in brackets, in addition to the current flow rate (in slpm = standard liters per minute). For the calculation of the suction section, a standard suction hose with 5mm inner diameter is assumed.



If the supplied gas volume is too low (< 0.30slpm) or in case of an interruption of the internal motor circuit, a visual and acoustical alarm will be emitted via the alarm system of the G999 gas measurement device. In addition to that, the message "PUMP Flow error!" will be displayed on the screen. A clogging of the gas path to the pump might be the cause for the malfunction. The hose is eventually pinched off or the filter is clogged. The problem needs to be fixed so it can start operating properly.



Caution: In case of a flow error, a proper measurement operation is no longer guaranteed.

2.2.7.3 Minimum pumping time

Gas samples are sucked e.g. from wells, rooms or channels by means of a hose with or without the GfG telescopic suction pipe. Since the response time largely depends on the inner volume of the suction device, its length should be kept as short as possible. The following rule applies for the minimum pumping time (t_{\min} in seconds):

$$t_{\min} = 10s + 3s/m * L_{\text{Schl}} + t_{\text{Tele}}$$

L_{Schl} = Hose length in meters with an inner diameter of 5 mm

t_{Tele} = 10s with GfG telescope, 0s without telescope

2.2.8 Use of the flash light

The integrated flash light can be switched on by long time pressing the left button (about 3 seconds) or switched off (press briefly). It is reasonable to use the flash light e.g. if the device is lowered onto a sewer shaft or if it is used as a safe light source in dark potentially explosive areas.

2.2.9 Display lighting

The display lighting is switched on by pressing any key for about 10 seconds and then it will automatically switch itself off. If the battery is relatively heavily discharged, the display lighting will no longer be switched on when pressing a key.

2.2.10 Recording of measurement data with the data logger

The measurement data can be recorded on the G999 with an internal data logger. No special activation of the data logging is required.

30,000 measuring points each can be recorded for up to 12 different measured values and other information. This includes date, time, measuring point, alarm triggering and special events.

In the menu item "data logger" of the service menu it is possible to set different functions of the data saving. It is possible to select the recording of average values, peak values or instantaneous value as well as the recording interval between 1 second and 60 minutes. The memory type is set to a ring memory at the factory. I.e. the oldest measured values will be overwritten as soon as the data logger is full. Measured data can be read with the help of a test station TS888/999 and a docking station DS400. The configuration of the data logger can be modified with the operating menu.

2.2.11 Influence of oxygen and interference gases

It is necessary to pay attention that the measurement for gas and / or vapour concentrations in the measurement range below 100% LEL can no longer exactly be performed, if the oxygen concentrations are at the same time less than 10 Vol%. In this case, the oxygen which is necessary for the "catalytic combustion" is missing for the heat tone sensor. If the oxygen sensor would measure such a low concentration, question marks "???" will be displayed instead of the measured value in %LEL. If the oxygen concentration would increase above 10 Vol.%, the measured value will be displayed correctly.

The Ex approval does not apply for the use of the device in an oxygen-enriched atmosphere.

Certain substances, which are designated as "Sensor or catalytic toxin" in the technical vocabulary, can impair the catalytic combustion sensor (CC) with regards to its signal behaviour. The "sensitivity", i.e. the ability of the sensor to emit signals, decreases. Substances of this kind are for instance sulphur, lead and silicon compounds.

2.2.12 Peculiarities when monitoring in the LEL range

For the monitoring of the LEL range, the G999C can be equipped with a sensor, which works according to the catalytic process (CC). Due to the measurement method, the G999C measured values in the LEL range cannot be distinguished from values in the increased Vol. % range (e.g. >20 Vol.% CH₄). Furthermore, the sensor would be damaged by concentrations above 110%LEL. In order to avoid such a damage, the sensor will be switched off if gas concentration above 110%LEL is being detected. Only by pressing the button **RESET** and confirming the question "Fresh air?" by pressing the button **YES** the sensor will be switched on again.

At an oxygen concentration of less than 10 Vol.% it would be no longer possible to measure flammable gases and vapours with the catalytic process (CC) without errors. Please find more details about this topic in the chapter "Influence of oxygen and interference gases".

2.2.13 HI% measurement of methane or natural gas

In the normal measurement operation, it is possible to measure methane (CH₄) in the range from 0...100% LEL with a catalytic combustion sensor or an infrared sensor. In this operating mode, all preset gas alarm thresholds are being monitored.

If the device has been equipped with a special HI%-IR sensor (MK245-1 or MK249-8), even higher concentrations of up to 100Vol% CH₄ can be measured. By simultaneously pressing the left and centre button, the system changes over to the HI% range. In this operating mode no gas alarms are being monitored. Besides the deactivated gas alarm, the readiness signal and, if applicable, also the catalytic combustion sensor will be switched off. At the top left a **HI%** icon is displayed on the screen. Then, the measured value of the infrared sensor will be displayed in Vol% CH₄ and afterwards the screen is empty at the position of the catalytic measured value. However, the pressure dependency of the IR sensor which are indicated in the sensor specifications need to be complied with.

If the gas concentration is less than 5Vol% CH₄, it is possible to change back to the %LWL range for monitoring by pressing the left and centre button once again. By monitoring the gas alarm thresholds, the readiness signal will be reactivated and, if applicable, the catalytic combustion sensor will be switched on again.

2.3 Service mode

Access the service mode by pressing the centre button for about 3 seconds long **RESET**. In the service mode it is possible to set the G999 by modifying the program parameters. Some menu items can only be accessed via an access code "0011". The access code prevents that important functions might be accidentally modified or modified by unauthorised persons. An alarming cannot be performed in the service mode.

The main menu is the first menu item in the service mode.

2.3.1 Main menu

Menu control: The individual key functions will always be displayed by the labelling via the individual buttons on the screen.




Left button = Scrolling one menu item downward
Centre button **SELECT** = Choosing the highlighted menu item
Right button **DETECT** = Back to the measurement operation

The individual menu items in the main menu are:

2.3.1.1 Place – Choice of a measuring point



From a table stored in the device, it is possible to select one of 100 possible places. All table entries can only be edited with a PC. In a table entry it is possible to save up to 15 letters / figures, which are saved as "**Job site**" in the G999.




By pressing the left and centre button a stored place is being selected. The choice is automatically completed, when the selected value is confirmed with the right "Back" button.

2.3.1.2 Name – Choice of a device user



From a table stored in the device, it is possible to select one of 20 possible entries. All table entries can only be edited with a PC. In table entries it is possible to save up to 15 letters / figures, which are saved as "**Identification**" in the G999.




By pressing the left and centre button stored user is being selected. The choice is automatically completed, when the selected value is confirmed with the right "Exit" button.

2.3.1.3 AutoCal – Menu for AutoCal adjustment




In the menu item AutoCal several sensors can be simultaneously adjusted with fresh air (ZERO) or test gas (KAL). Except from the CO₂ sensor, all sensors can be adjusted with fresh air without any further settings. When adjusting with test gas (KAL) the sensors need to be released depending on the used test gas / mixture. (Also refer to the paragraphs "AutoCal air . . ." and "AutoCal gas . . .")

The menu item AutoCal can be selected in the main menu. However, it is also automatically displayed as soon as the calibration cap "Smart Cap" or the charger cap "smart Charger Cap" is put on.






Then, the following functions can be chosen:

AIR = AutoCal adjustment with fresh air
GAS = AutoCal adjustment with test gas
EXIT = Back to the main menu



AutoCal adjustment with fresh air has been successful.




AutoCal adjustment with test gas mixture has not been successful.
(e.g. Due to wrong test gas concentration)


An AutoCal adjustment with fresh air is only performed if the sensor reading of the set point 0.0 (except for O₂) does not deviate more than $\pm 10\%$ from the measuring range or if the set point 20.9Vol.%O₂ does not deviate more than $\pm 5.2\text{Vol.}\%O_2$. An AutoCal adjustment with test gas is only performed if the sensor reading of the "Cal.Gas" set point (in the sensor menu "Calibrate") does not deviate more than 25%. In case of larger deviations, the corresponding sensor will then be marked with "Error" in the subsequently indicated AutoCal report. In this case, adjust the sensor in the sensor menu "Zero" or "Calibrate" or with the docking station.

The adjustment can be performed in the diffusion mode with fresh air exempt from measuring gas. However, no ambient air should be used for the zero point adjustment of the CO₂ sensor, since the ambient air always contains a small portion of carbon dioxide (CO₂) which would then result in wrong CO₂ measured values. For this reason, the zero point of the CO₂ sensor should only be adjusted in the sensor menu "Zero" or with the docking station with CO₂-exempted zero gas. It could be e.g. synthetic air, 100Vol.%N₂ or specially purified air (CO₂-free). Zero gas (air exempted from measurement gas) and test gas can be supplied via the calibration cap "Smart Cap" or the charger cap "Smart Charger Cap" with a volume flow from 0.5 to 0.6 l/min.

2.3.1.4 Sensor overview





or




The sensors which are represented in the overview are located in the corresponding plug-in locations of the device.

Display of the alarm settings as well as date and status of the last calibration



The data of the last three sensitivity adjustments can be displayed in the sensor menu "Calibration data". The status display indicates if they have been successful (✓) not faulty (✗).


Sensor information



In this menu item, specific information for each individual sensor are displayed:

- ID = Number of the measuring chamber
- SN = Serial number
- MB = Measuring range
- TB = Temperature range
- BD = Operating time of the sensor, e.g. 125 of 791 days

2.3.1.5 System information



In the system menu item **Information** you will find information about the device type, the firmware version, the serial number of the device.

2.3.2 Service menu

Access the service menu by selecting the main menu item **Service**. In the service menu it is possible to set the G999 by modifying the program parameters.

The menu items can only be accessed via an access code "0011". The access code prevents that important functions might be accidentally modified or modified by unauthorised persons. An alarming cannot be performed in the service mode.



ABC

= Go to the next letter in the alphabet


<<>>

= Confirm letters (The cursor automatically skips to the next position). By long pressing the key, the last entry will be deleted, the cursor will skip one position back.

012↑↑

= Go to the previous letter in the alphabet



After having entered the code 0011, the following will be displayed:



In the menu item **System** it is possible to perform general settings (refer to the chapter "System menu"). In the menu item **Sensors** it is possible to set sensor-specific functions (zero point and sensitivity adjustment). It is possible to retrieve information or to set alarm thresholds.


By pressing the button **DETECT** you quit the service menu and go back to the measuring mode.

2.3.2.1 System menu for system settings




2.3.2.1.1 Bump test


The functional test (inspection of the sensor values and alarms) can be easily and rapidly performed with the docking station DS400. The functional test is performed automatically, the intervals for the functional test will be stored in the G999. The functional test interval will be activated in the docking station after the first functional test.



Interval of the functional test is not activated




Interval of the functional test is activated; the next functional test is immediately due



Functional test on January 15th, 2018 was correct
Next functional test will be due 7 days later

2.3.2.1.2 Sensor adjustment (zero point + calibration)

The sensor adjustment (zero point and sensitivity adjustment) can be easily and rapidly performed fully automatic with the docking station DS400. The intervals for the sensor adjustment will be saved in the G999 and activated from the docking station after the first sensor adjustment.



Sensor adjustment on September 07th, 2017 was correct
Interval for the sensor adjustment is not activated

Calibration		
last	07.09.2017	✓
next	14.02.2018	-
Interval	29 days	
↓↓	↑↑	EXIT

Sensor adjustment on September 07th, 2017 was correct
Next sensor adjustment will be due 29 days later

2.3.2.1.3 Inspection

It is possible to enter a date in order not to forget the date for the next maintenance or inspection; the G999 will automatically trigger an alarm if this date is exceeded. After having exceeded the date, the G999 will inform the user that an inspection needs to be performed as soon as the device is switched on.

To do so, it is necessary to select first **Inspection** in the service menu.

Inspection		
Next date:		
YYYY-MM-DD		
2018-01-06		
>>	SELECT	EXIT

It is possible to first select which parameter needs to be changed (year, month and day):

EXIT	= Back to the system menu
SELECT	= Selecting the parameter to be flashing
>>	= Change over to the next parameter

Inspection		
Next date:		
YYYY-MM-DD		
2018-01-06		
↓↓	EXIT	↑↑

The following options are available in order to modify a parameter:

↓↓	= Reduce value
EXIT	= Confirm value
↑↑	= Increase value

2.3.2.1.4 Time

The device has a clock for date and time. The summer and winter time is not automatically changed over. The clock is buffered by a lithium cell, which is designed for a useful life of 20 years.

Time menu		
YYYY-MM-DD hh:mm:ss		
2018-01-15 17:11:19		
>>	SELECT	EXIT

In the **Time menu** the corresponding flashing parameter is selected with

SELECT	= Select.
>>	= Skip to the next parameter.
EXIT	= Go back to the system menu.

Time menu		
YYYY-MM-DD hh:mm:ss		
2018-01-15 17:11:29		
↓↓	EXIT	↑↑

The following options are available in order to modify a parameter:

↓↓	= Reduce value
EXIT	= Confirm value
↑↑	= Increase value

2.3.2.1.5 System options

If "**System options**" is selected in the service menu, the following will be displayed:

System options		
Language	12	
Contrast	103dB(A)	
Volume	off	
MotionAlert	off	
Radio (868MHz)	on	
Tolerance band	on	
↓↓	SELECT	EXIT

- **Language** (language options)
- **Contrast** (setting the contrast values)
- **Volume** (103dB(A), 90dB(A), 0dB(A))
- **Motion alarm** (on/off)
- **Radio** (on/off and setting the radio ID)
- **Tolerance band** (on/off)
- **Vibrator** (on/off)
- **Startup+AutoCal** (on/off)

System options		
Volume	103dB(A)	
MotionAlert	off	
Radio (868MHz)	off	
Tolerance band	on	
Vibrator	on	
Startup+AutoCal	off	
↓↓	SELECT	EXIT


Switch tolerance band on/off

In the measuring mode, the G999 suppresses low measured value fluctuations in the range of the zero point on sensors for toxic and flammable gases. In case of the oxygen measurement, low fluctuations about 20.9Vol% O₂ (fresh air range) will be suppressed. In order to avoid skips, the display value will be adjusted to the double value of the tolerance band up to the real measured value.

This tolerance band is activated by the manufacturer, but it can generally be switched off as well. For this purpose, it is necessary to enter the shortcut <REAL> for the deactivation or the shortcut <BAND> for the activation instead of the access code. Please find detailed information about the size of the tolerance band in the chapter "Sensor types and measuring ranges".

2.3.2.1.6 Sensor choice – Activation / deactivation of sensors

Each sensor can be individually switched on or off for the measurement. This function will always be used if a gas shall not be measured or if a sensor is taken out of the device without replacing it.



On = Sensor active

Off = Sensor inactive

If no (gas) is indicated behind the sensor, the sensor is not available or it is not being identified.



= Scroll downward to the next sensor


On/Off

= Activate / deactivate the corresponding sensor

EXIT

= Back to the service menu

2.3.2.1.7 AutoCal air – Sensor release for AutoCal adjustment



Here it is possible to set which sensors should be used for the automatic adjustment with fresh air.

Except for the IR sensor for CO₂ by default all sensors are set to "ON" and are thus released for the automatic fresh air adjustment.



= Scroll downward to the next sensor


On/Off

= Adjustment / Non-adjustment of the sensor in the AutoCal program

EXIT

= Back to the service menu

2.3.2.1.8 AutoCal gas – Sensor release for AutoCal adjustment



Here it is possible to set which sensors should be calibrated for the automatic adjustment with test gas. By default, all sensors are set to "Off". If several sensors need to be adjusted simultaneously with a test gas mixture, these sensors can be selected here.



= Scroll downward to the next sensor

On/Off

= Adjustment / Non-adjustment of the sensor in the AutoCal program

EXIT

= Back to the service menu

2.3.2.2 Sensor menu for sensor settings

The following functions refer to the individual sensors in the G999. In the sensor menu, each sensor can be selected individually. Then, the settings apply for each selected sensor.

For the description of the functions of the sensor-specific settings the CH₄ sensor resp. the O₂ sensor are mentioned as an example. However, the setting options apply for all sensors in the same way.



Input options:



= Changing over to the next sensor

SELECT

= Selecting the sensor

EXIT

= Back to the service menu



The following settings are available for each sensor:

Zero

= Adjusting the zero point

Calibrate

= Adjusting the sensitivity

Alarms

= Setting the alarm thresholds

Calibration data

= Data and status of the last calibration and zeroing

Information

= Sensor information: MK number, serial number, measuring range, temperature range

Unit and

= Selecting the CH₄ unit to be displayed (%UEG / Vol%)

Type of gas

or selection of the type of gas to be displayed



= Changing over to the next menu item

SELECT

= Selecting the menu item

EXIT

= Back to the service menu

2.3.2.2.1 Zero – Adjusting the zero point

When adjusting the zero point, the sensors should be gassed with air exempt from measuring gas or the carbon dioxide and the oxygen sensor (*1) with 100Vol.% nitrogen. In this case, the zero gas can be supplied by means of the "Smart Cap" or the "Smart Charger Cap" with a flow from 0.5 to 0.6l/min. In order to adjust the zero point, it is necessary to select the sensor menu item "Zero". Then, the following will be displayed:

```

=====CH4(CC)-ZERO=====
Readout:  0.0 %LEL
ZeroGas:  0.0 %LEL
START    GAS    EXIT
  
```

START
GAS
EXIT

- = Starting the zero point adjustment
- = Inputting the zero gas concentration
- = Back to the "CH₄menu"

Generally, the zero gas is 0.0 so that it is not necessary to modify this concentration. However, in special cases, the zero gas concentration can be slightly raised after having pressed the button GAS. After having input **GAS** the following screen will be displayed:

```

=====CH4(CC)-ZERO=====
Readout:  0.0 %LEL
ZeroGas:  0.0 %LEL
START    GAS    EXIT
  
```

↓
EXIT
↑

- = Reducing the zero gas concentration by one unit
- = Confirming the value and back to the menu item "Zero"
- = Increasing the zero gas concentration by one unit

By inputting **Start** the zero point adjustment is being started:

```

=====CH4(CC)-ZERO=====
Readout:  0.0 %LEL
ZeroGas:  0.0 %LEL
ABORT
  
```

ABORT

- = Cancelling the adjustment and changing over to the "CH₄" menu.

If a constant measured value is registered after a stabilisation time of 100 seconds, the adjustment will be performed and conformed by pressing the button "OK". For CC, IR and O₂ sensors the stabilisation time is a bit longer but generally limited to 3 minutes.

For (*1): The zero point adjustment of the oxygen sensor will be performed with 100Vol.% oxygen at the factory. For the monitoring of the usual alarm thresholds of ≥17Vol.%O₂ no readjustment of the user is being required. In this case, it is sufficient to adjust the sensitivity.

2.3.2.2.2 Calibrating – Sensitivity adjustment

The gas sensitivity of the sensor is adjusted for the calibration. Before performing the sensitivity adjustment, a zero point adjustment needs to be performed. A corresponding test gas is required for the sensitivity adjustment. Test gases are e.g.:

Measuring range	Test gas
TX	Carbon monoxide (CO), hydrogen sulphide (H ₂ S) or other gases
OX	Fresh air or test gas with 20.9 Vol.-% oxygen (O ₂) in nitrogen (N ₂)
EX	Methane (CH ₄), propane (C ₃ H ₈) or any other flammable gases (*2)

The test gases to be used can be learned from the test log. For the sensitivity adjustment, the concentration of the test gas should amount to from 30% to 70% of the measuring range end value. However, for IR sensors with measuring ranges of >5Vol.CO₂ the concentration of the test gas has to amount to from 25% to 75% of the measuring range end value. The test gas can be supplied with the "Smart Cap" or the "Smart Charger Cap" with a flow from 0.5 to 0.6l/min.

In order to adjust the sensitivity, it is necessary to select the sensor menu item "Calibrate".

```

=====O2(EC3)-SPAN=====
Readout:  20.9 Vol%
Cal.-Gas:  20.9 Vol%
START    GAS    EXIT
  
```

START
GAS
EXIT


- = Starting the sensitivity adjustment
- = Inputting the test gas concentration
- = Back to the "O₂" menu

By inputting the **GAS** the test gas concentration can be set in the range from 10 to 105% of the measuring range end value:



- = Reducing the test gas value by one unit
- = Increasing the test gas value by one unit
- = Confirming the value and back to the "O₂" menu

However, by inputting **Start** the sensitivity adjustment is being started:



- = Cancelling the adjustment and change over to the "O₂" menu.

If a constant measured value is registered after a stabilisation time of 25 seconds, the adjustment will be performed and confirmed by pressing the button "OK". Generally, the stabilisation time is limited to 3 minutes.

For (*2): The sensitivity adjustment of sensors which measure certain flammable gases in the %LEL range, such as e.g. n-hexane, n-nonane or similar "heavy" vapours, is not unproblematic. Apart from the availability of such a test gas, it has to be assumed with a long stabilisation time in the range of several minutes for the gas supply. Alternatively, the sensitivity adjustment can be performed with a suitable reference gas (e.g. propane). The IR sensor MK249-8 can be adjusted e.g. with a reference gas of 0.85Vol% C₃H₈ (propane) to 67%LEL n hexane or 80%LEL n nonane. The cross-sensitiveness for such sensors are indicated in the chapter "Sensor specifications".

2.3.2.2.3 Alarms – Alarm setting


The G999 has 3 limit value alarms for the non-toxic gases (O₂, CH₄) each, for the toxic gases (e.g. H₂S, CO, CO₂) there are 2 limit value alarms each. The alarms are triggered if the gas concentration exceeds or falls below the corresponding limit value. An alarm can additionally be emitted for the toxic gases if the long-term and the short term value (LZW and KZW) are being exceeded.

After having selected the sensor menu item **Alarms** the following screen is displayed (here: Selecting O₂):



- = Scrolling downwards
- = Selecting the menu item
- = Back to the sensor menu

After having selected the alarm limit value (in the example: Alarm 1) it is possible to enter the value:



The selected alarm limit value flashes and can only be changed, if:






- = Reducing the alarm value by one unit
- = Back to the sensor menu
- = Increasing the alarm value by one unit

With the exception of %LEL measuring ranges all limit values can be freely set or completely deactivated (0 or "---") over the whole measuring range. For %LEL measuring ranges, the limit values can be set to up to maximum 60%LEL.



2.3.2.2.4 Calibration data

In this menu item, the data of the last calibration will be displayed. It is a pure information display.




2.3.2.2.5 Information

The individual data of the smart GfG sensors which are built-in this device, have been displayed here.



2.3.2.2.6 Measuring range

Under the menu item Measuring range, different pre-defined measuring ranges are listed for smart GfG sensors. They can be selected.



In this menu item (here CC sensor) it is possible to select the type of gas to be displayed or to set the CH₄ unit to %LEL or Vol.%. The volume concentration in brackets corresponds to the final value of the measuring range. Hereby it is possible to set the measuring range to the country-specific LEL value.

If the unit or the type of gas has been changed, the device needs to be restarted after quitting the service program, before performing a functional test or an AutoCal adjustment with a docking station.

2.3.2.3 Data logger settings

In the menu item **Data logger** it is possible to make different settings:

Complete - Deleting the data from the data logger (display of the memory usage)

Mode - Selection of instantaneous values, mean values or peak values

Interval - Interval of the data logging (selectable from 1 second to 60 minutes)




The parameter **COMPLETE** indicates how much capacity of the data logger has been completed.



ERASE

- = Scrolling downward to the next parameter
- = Deleting the data. A security query will follow "Delete data?". Confirm by pressing the button **YES** (right button), cancel by pressing the button **NO** (left button)
- = Back to the main menu



EXIT

If the parameter **Mode** is selected by pressing the button **CHANGE**, it would be possible to choose between the instantaneous value, mean value and peak value (Peak). After having input **EXIT** the system will skip back to the logger menu. The selected mode will be taken over.



Interval: The interval of the data logging can be selected by pressing the buttons on the left and right from 1 second to 60 minutes.

The data of the data logger can be read with the help of the charging tray or of the charging cap and an optional USB adapter cable and be transferred to a PC.

2.4 Power supply

The G999 has an NiMH battery module. In this supply module, the battery is an integral part of the back of the housing. A dangerous dendrite growth, as e.g. in lithium-polymer or lithium-ion batteries are excluded in the G999 battery module.

2.4.1 Charging the battery



Caution:

The device must not be charged in potentially explosive atmospheres.
The charging contacts must not get dirty. (Refer to the chapter "Maintenance")

The battery module in the G999 can be charged in the **charging tray**. Perfect functioning is only guaranteed if the charging tray is lying or is fixed horizontally and the mounting bracket is correctly clammed in. Caution: Do not mount vertically!

The charging tray will be supplied by a plug-in power supply made by the company GfG or alternatively via a vehicle charging cable made by the company GfG. The charging tray limits the charging voltage for the G999 to max. 9V. The charging process is subdivided in normal and trickle charging. The green LED signals the operational readiness of the charging tray. The green LED indicates the charging process (Off: No device in the charging tray, constantly illuminated: Charging, Flashing: Trickle charging).

Ensure that the charging process will be indicated by the yellow LED and on the display after having inserted the G999 into the charging tray and closing the mounting bracket (otherwise there might possibly be contact problems).

In case of a completely discharged battery, the charging process will take about 6 to 7 hours. Then, the charging tray will automatically switch over to the trickle charging so that an overloading of the battery will be excluded. Both states of charge will be displayed on the screen of the G999. After having switched over to the trickle charge, the battery will have at least 98% of its capacity. In order to attain a capacity of 100%, the battery module needs to be charged another 2 hours with trickle charging.

With the help of the charging tray and an optional USB adapter cable, the data of the G999 data logger can be read and transferred to a PC.

In order to permanently maintain the capacity of the NiMH battery, make sure that the battery can only be charged by using the charger depending on the useful life and frequency and the charger is not used as a storage place for weeks for the gas measurement device. Please find recommendations in the following table for the charging depending on the device usage.

	Device usage	Recommendation for the charging of the battery
1.	Daily for more than 3h	Charge after use
2.	Daily for less than 3h	Charge every 2nd or 3rd day
3.	Once per week	Charge 1 day before the next use
4.	Once per month for more than 3h	Charge after use as well as 1 day before the next use
5.	Once per month for less than 3h	Charge 1 day before the next use
6.	Once per calendar quarter or rarer	Charge after use as well as 1 day before the next use



Charging tray with mounting bracket

For 4,5,6: If the device is rarely used, then the battery needs to be charged after use, since one part of the sensor electronics also needs to be supplied with energy even when the device is switched off. If the device has not been used for a very long period of time and the battery is completely discharged, then the device needs to be recharged about 1 day before the next use. A normally discharged battery will generally be charged to 98% of its normal capacity within about 6 hours charging mode. After another 2h trickle charging mode, the battery will be charged to 100% of its normal capacity. If in spite of the completely charged battery the normal device service life would not be attained, this might be caused due to the "lazy battery effect" (effect of the inertia of the battery). At this, the discharge behaviour changes in such a way that in

spite of the completely charged battery the battery icon is empty relatively quickly and the device can nevertheless be operated for a long time.

2.4.2 Lazy battery effect on the NiMH battery and its removal

On the NiMH supply units, the "lazy battery effect" and thus a reduction of the service life of the device might occur due to temperature influences above 50°C, after longer non-use, due to unfavourable device use or due to wrong charging behaviour. This may occur if the battery of the device has never been completely discharged or if the battery is charged too often or too long. It has to be avoided to start the charging process several times per day and that the device is permanently deposited in the charger for several days or weeks. The "lazy battery effect" can often be remedied by completely discharging the NiMH battery. However, in order that the battery would not be completely discharged, the device must not be manually switched off.

2.4.3 Changing the battery module



Caution: The device must not be opened in potentially explosive areas and therefore the battery module is not being changed. The battery is an integral part of the back of the housing, it must only be replaced outside of potentially explosive areas and only by a NiMH battery module of the same type.

Before replacing the battery module, the device needs to be switched off. In order to remove the supply module, the six screws at the back of the device need to be unscrewed and the whole module needs to be pulled off to the rear.

3 Annex

3.1 Maintenance

Soiling of the device housing can be removed using a cloth dampened with water. Do not use solvents or cleaning agents! Particularly make sure that the outer charging contact surfaces of the G999 and the charging contact pins of the charging adapters are clean. In case of bad/incorrect contacting of the charging adapter, the NiMH battery will only be charged incompletely or not at all.

3.2 Maintenance and inspection

The maintenance and inspection includes a regular review and adjustment of the sensitivity and of the zero point. Moreover, the functioning of the device needs to be checked. Gas warning devices can behave in different ways depending on the environmental conditions. Thus, it is important to perform a test and an adjustment, if applicable, independent from the maintenance works (refer to the DIN EN 60079-29-2 paragraph 9.2 as well as the DGUV Information 213-057 (T 023) and DGUV Information 213-056 (T 021) of the BG RCI in Germany). This test includes the following inspections:

- Visual inspection regarding mechanical damages
- Visual inspection of the gas entry
- State of charge of the battery
- Display with zero gas and with test gas as well as alarm triggering

The response behaviour of oxygen sensors can be checked with a suitable test gas (<18Vol.% O₂) and with the help of the docking station, of the calibration flap "Smart Cap" or of the charger cap "Smart Charger Cap". In the simplest case, the response behaviour can also be checked with slowly exhaled air.

3.3 Maintenance - Repair

The DIN EN 60079-29-2 „... gas measurement devices – selection, installation, use and maintenance of devices for the measurement of flammable gases and oxygen“, the DIN EN 45544-4 „... Electrical devices for the direct detection and direct concentration measurement of toxic gases and vapours, Part 4: Guideline for the selection, installation, use and maintenance“ as well as the corresponding national sets of rules need to be considered.

In the sense of the “Explosion protection directive”, the “BGR 500, Chapter 2.33” (formerly: Accident prevention regulations (UVV) gases), the maintenance includes the maintenance, inspection and repair of gas warning units. The applicable measures are described in the DGUV Information 213-057 (T 021) and 213-056 (T 023) the BG RCI. The functional test has to be performed before the first use and at least every 4 months and includes:

- Position of the zero point
- State of charge of the battery
- Diffusion paths
- Display with zero gas and standard test gas, if applicable, adjustment
- Alarm signal triggering, e.g. with alarm test gas
- Constantly amplified signal with standard test gas
- Setting time

The test has to be performed by an expert and a written confirmation about the result has to be available.

Generally, the restoration of the G999 has to be performed according to the instructions of the manufacturer by using original spare parts for the maintenance.

3.4 Calibration device

The device has to be supplied with test gas in order to control the sensitivity of the display. The diffusion openings can be covered with the help of the “Smart Cap”, so that the test gas can be supplied to the sensors with a flow from 0.5 to 0.6l/min. Alternatively for certain test gases, this inspection can also be performed with the docking station DS400.

Caution: Test gases, in particular toxic gases may pose hazards. Make sure that test gases are not inhaled. Working places, where devices are calibrated with test gas, need to be sufficiently ventilated depending on the type of gas, concentration and gas quantity. In particular cases, a gas extraction or a gas discharge is suitable. The safety notes on the test gas bottles as well as the safety data sheets of the test gases need to be observed in any case.

3.5 Inspection with the docking station DS400

The functional test required in the DGUV Information 213-057 (T 023) and 213-056 (T 021) as well as the adjustment of the G999 can be easily and rapidly performed with the docking station.



The functional test will be automatically started and performed fully automated. The effective time for a functional test amounts to about 20 seconds. The adjustment (sensor adjustment) will be started at an individual push of a button and completed within a few minutes. A green or red LED will indicate the test result. The detailed values are displayed on the device screen (functional test report, AutoCal air report, AutoCal gas report). No PC is required to perform the functional tests and the adjustment; all relevant data will be automatically saved on an SD card which is inserted in the docking station.

The first time, the functional test of the G999 needs to be performed; the interval for the functional test and the adjustment can be automatically activated on the docking station.

Before using the docking station, it is necessary to read and follow its operating instructions.



3.6 Malfunction, cause, remedy

	Malfunction / Message	Cause	Remedy
1.	Simultaneously flashing alarm LEDs and display off	Insufficient voltage supply Hardware or program execution error	Charge battery Call the GfG service
2.	Permanent "Boot loader" with red display lighting	Program memory defective	Transfer Firmware to the device Call GfG service, if necessary
3.	"ERROR! RAM"	Working memory defective	Switch device off and on Call GfG service, if necessary
4.	"ERROR! EEP"	Device parameter memory defective	
5.	"ERROR! BAT"	Battery voltage metering defective	
6.	"ERROR! ALG"	Program execution error / Algorithm	
7.	"Clock clip does not work!" "Time reset to ..."	Hardware defect	Acknowledge message Call GfG service, if necessary
8.	"Reset time to ..."	Clock not set or buffer battery is empty	Acknowledge message, set time Call GfG service, if necessary
9.	"Sensor defective!"	Sensor defective or not available	Switch device off and on Call GfG service, if necessary
10.	"Data incorrect!"	Sensor data are incorrect	Switch device off and on Call GfG service, if necessary
11.	"Reconnect sensor to EC1!"	EC sensor is connected to the wrong slot	Open device, reconnect sensor, then switch the device on again
12.	"Reconnect sensor to EC2 or EC3!"		
13.	"Sensor not available. Deactivate sensor in the system menu!"	Sensor not available.	Acknowledge message and switch off sensor in the service program Call GfG service, if necessary
14.	"CHECK ALARMS"	Sensor was replaced by another type	Check alarm setting in the service program and change it, if necessary
15.	"Gas type is not supported"	Gas type is not supported by the device or old Firmware version	Remove sensor perform Firmware update, if necessary
16.	"No sensors"	No sensors activated in the service program	Activate available sensors in the service program
17.	Gas display "START" ("STRT")	Sensor is still in the activation phase	Wait for some seconds
18.	Gas display "????"	Measuring with CC sensor is not possible, since oxygen display <10Vol%	If this occurs with fresh air, it is necessary to adjust or replace the oxygen sensor
19.	Gas display "----" / Error	No gas display, since the sensor is defective or the sensor data are incorrect	Deactivate the sensor in the service program Call GfG service, if necessary
20.	Gas display 	Measured value underrange Clearly falling below the measuring range	Perform zero point adjustment
21.	Gas display 	Measured value over range/excess available gas concentration is too high or high cross sensitivity (for EC sensor) or protective circuit activated (for CC sensor)	Quit range of high gas concentration and acknowledge message for the CC sensor and confirm in the fresh air range
22.	Gas display "FAULT" ("FLT")	IR sensor signal is incorrect	If this happens repeatedly Call GfG service
23.	Gas display "TEMP" or "TEMP ERROR"	Sensor is operated outside the specified temperature range or hardware defect at 0°C < Ta < 30°C	Go to a normal environmental temperature range Call GfG service, if necessary
24.	Gas display "POWER" or "POWER ERROR"	Energy supply of the sensor is disturbed	If this happens repeatedly Call GfG service
25.	Gas display "P+T"	See gas display "TEMP" and "POWER"	See above
26.	"Gas concentration is too high!"	When changing from the HI% range to the %LEL range the gas concentration is still above 5Vol%	Wait until the gas concentration has reduced to less than 5Vol% and repeat switchover.
27.	"No sensors released for AutoCal air (gas)"	No sensors released for the automatic fresh air or test gas adjustment	Release for the automatic adjustment in the service program Sensor(s)
28.	"Zeroing failed measured value too high" (too low)	Possibly measuring gas available or too positive (negative) zero point deviation	Perform zero point adjustment in the environment exempt from measuring gas / Call GfG service, if necessary
29.	"Calibration failed Measured value too low" (too high)	Wrong test gas concentration or sensor sensitivity too low (too high)	Check test gas and set point Call GfG service, if necessary

30.	"Zeroing (calibration) failed Signal cannot be detected"	Extreme sensor signal deviation or hardware defect	Repeat process and call GfG service, if necessary
31.	"Saving failed"	Parameters cannot be saved when quitting the service program	Switch device off and on, then repeat the settings in the service program Call GfG service, if necessary

3.7 Accessories and spare parts

	Description	Order No
1.	G999C NiMH Battery pack A21 (back housing)	1990301
2.	G999E NiMH Battery pack A21 (back housing)	1990302
3.	G999P NiMH Battery pack A21 (back housing)	1990303
4.	G888/G999 SMART CAP (calibration cap)	1990210
5.	G888/G999 SMART CAP with USB cable (calibration cap and data transfer)	1990211
6.	DIC888/999-B Charging tray with brackets and EU plug-in power supply	1990221
7.	DIC888/999-B Charging tray with brackets and vehicle charging cable	1990222
8.	DIC888/999 USB interface cable	1990229
9.	DS400 Docking station for G888/G999-D with EU plug-in power supply	1990231
10.	DS404 Docking station for G888/G999-D with EU plug-in power supply	1990236
11.	TS888/999 Test station without fitting without plug-in power supply	1990240
12.	TS888/999 Test station with fitting without plug-in power supply	1990241
13.	TS888/999-DIC Test station with charging function w/o fitting without plug-in power supply	1990245
14.	TS888/999-DIC Test station with charging function with fitting without plug-in power supply	1990246
15.	Spare sensors refer to the chapter "Sensor types and measuring ranges"	

The spare parts and the accessories need to be stored at an environmental temperature from 0° to 30°C. The storage time must not exceed 5 years. For NiMH supply units a shorter storage time of one year applies. The battery must be charged before the storage. If the device might be stored for more than ½ year, the battery should be removed.

3.8 Indications regarding the environmentally friendly disposal

According to section 11 of the General Terms and Conditions of the company GfG, the purchaser of the device agrees to dispose of the device or device components in an environmentally sound manner in line with sections 11 and 12 of the German Electrical and Electronic Equipment Act (ElektroG). If desired, GfG in Dortmund, Germany, can also carry out correct disposal.

3.9 Sensor types and measuring ranges

The spare sensors need to be stored at an environmental temperature from 0° to 30°C. The storage time must not exceed one year. For electrochemical sensors a shorter storage time of ½ year applies. When storing oxygen sensors, the service life to be expected will be reduced. When storing the spare sensors, make sure that the environmental atmosphere is not aggressive and free from sensor toxins.

Slot	Sensor type	Display range	Measuring gas and additional information	Order No
EC1	MK380-8	0 ... 500ppm 0 ... 100ppm	CO Carbon monoxide and H ₂ S hydrogen sulphide	1990710
EC1 EC2 EC3 EC4 (*E)	MK390-8	0 ... 10ppm (*1)	Cl ₂ Chlorine	1990725
	MK391-8	0 ... 2ppm	ClO ₂ Chlorine dioxide	1990730
	MK349-8	0 ... 2ppm	COCl ₂ Phosgene	1990800
	MK443-8	0 ... 500ppm (*1)	CO Carbon monoxide	1990705
	MK445-8	0 ... 100ppm (*1)	H ₂ S Hydrogen sulphide	1990700
	MK396-8	0 ... 2000ppm	H ₂ Hydrogen	1990785
	MK402-8	0 ... 1Vol. %	H ₂ Hydrogen	1990790
	MK403-8	0 ... 4Vol. %	H ₂ Hydrogen	1990795
	MK409-8	0 ... 50ppm (*1)	HCN Hydrogen cyanide	1990760
	MK412-3	0 ... 10ppm	HF Hydrogen fluoride (EU version)	1990765
	MK412-9	0 ... 10ppm	HF Hydrogen fluoride (resolution 0.5ppm)	1990766
	MK453-8	0 ... 300ppm (*1)	NH ₃ Ammonia	1990735
	MK454-8	0 ... 1000ppm(*1)	NH ₃ Ammonia	1990740
	MK458-8	0 ... 30ppm (*1)	NO ₂ Nitrogen dioxide	1990750
	MK383-8	0 ... 25Vol. %	O ₂ Oxygen (2 years)	1990715
	MK427-8	0 ... 25Vol. %	O ₂ Oxygen (3 years)	1990716
	MK353-8	0 ... 10ppm (*1)	PH ₃ Phosphine	1990770
	MK460-8	0 ... 20ppm (*1)	SiH ₄ Silane	1990780
	MK440-8	0 ... 10ppm (*1)	SO ₂ Sulphur dioxide	1990720
EC2 EC3 EC4 (*E)	MK379-8	0 ... 20ppm (*1)	C ₂ H ₄ O Ethylene oxide	1990775
	MK392-8	0 ... 30ppm (*1)	HCl Hydrogen chloride	1990755
	MK457-8	0 ... 100ppm (*1)	NO Nitrogen monoxide	1990745
PID (*P)	MK222-0	0 ... 2000ppm	iC ₄ H ₈ Isobutylene and other VOCs	1990980
CC (*C)	MK221-0	0 ... 100%LEL	Flammable gases and vapours (*2)	1990850
		0 ... 5Vol. %	CH ₄ Methane	
	MK221-1	0 ... 100%LEL	Flammable gases (*2) (increased contamination resistance)	1990851
		0 ... 5Vol. %	CH ₄ Methane (increased contamination resistance)	
IR (Infrared)	MK245-1	0 ... 5Vol. %	CO ₂ Carbon dioxide	1990920
		0 ... 100%LEL	Flammable gases and vapours (*2)	
		0 ... 5Vol. %	CO ₂ Carbon dioxide	
		0 ... 100%LEL	Flammable gases and vapours(*2)	
	MK248-8	0 ... 100Vol. %	CH ₄ Methane	Upon request
		0 ... 5Vol. %	CO ₂ Carbon dioxide	
		0 ... 25Vol. %	CO ₂ Carbon dioxide	
		0 ... 25Vol. %	CO ₂ Carbon dioxide	
	MK249-8	0 ... 100%LEL	Flammable gases and vapours (*2)	1990905
		0 ... 100%LEL	Flammable gases and vapours (*2)	
		0 ... 100Vol. %	CH ₄ Methane	
		0 ... 100Vol. %	CH ₄ Methane	

For (*1): The sensor can also be set to other measuring ranges (refer to the sensor specification)

For (*2): CH₄ Methane or one of the below mentioned flammable gases and vapours

For (*E): EC4 is only available in the G999E

For (*P): PID is only available in the G999P

For (*C): CC is only available in the G999C

Sensor type	Flammable gases and vapours
MK221-0	CH ₄ (methane), C ₃ H ₈ (propane), C ₄ H ₁₀ (butane), C ₅ H ₁₂ (pentane), C ₆ H ₁₄ (n hexane), H ₂ (hydrogen), C ₂ H ₂ (acetylene), C ₂ H ₄ (ethylene), CH ₃ O(methanol), C ₂ H ₅ O(ethanol), C ₃ H ₇ O(isopropanol), C ₄ H ₉ O(n butanol), C ₃ H ₆ O(acetone), C ₃ H ₇ O ₂ (methylacetate), C ₄ H ₉ O ₂ (ethylacetate), C ₄ H ₈ O(methylethylketone MEK), C ₇ H ₈ (toluene), C ₆ H ₁₂ O(methylisobutylketone MIBK), C ₇ H ₁₆ (heptane), C ₉ H ₂₀ (n nonane)
MK221-1	CH ₄ (methane), C ₃ H ₈ (propane), C ₄ H ₁₀ (butane), C ₅ H ₁₂ (pentane), C ₆ H ₁₄ (n hexane), H ₂ (hydrogen), C ₂ H ₂ (acetylene), C ₂ H ₄ (ethylene)
MK245-1 MK249-8	CH ₄ (methane), C ₃ H ₈ (propane), C ₆ H ₁₄ (n hexane), C ₉ H ₂₀ (n nonane), ETF (ethyl formate)

3.10 Sensor specification

MK221-0 Catalytic combustion sensor for flammable gases and vapours				
Measuring ranges:	0.0...100%LEL		0.00...5.00Vol.% CH ₄	
Resolution / tolerance band:	0.5 / ±2.5%LEL		0.02 / ±0.14Vol.% CH ₄	
Setting time:	t ₅₀ ≤ 10 sec	t ₉₀ ≤ 20 sec	@ CH ₄ (methane)	
	t ₅₀ ≤ 12 sec	t ₉₀ ≤ 30 sec	@ C ₃ H ₈ (propane)	
	t ₅₀ ≤ 25 sec	t ₉₀ ≤ 65 sec	@ C ₆ H ₁₄ (n hexane)	
Pressure (70)80....120(130)kPa:	max. ±5(7)%LEL or ±10% of the display		(regarding 100kPa)	
Humidity 0%...95% RH:	max. ±3%LEL or ±10% of the C ₃ H ₈ display		(regarding 0% RH @40°C)	
	or ±30% of the CH ₄ display		(regarding 0% RH @40°C)	
Temperature(-20)-10...+40(55)°C:	max. ±3%LEL or ±10(15)% of the display		(regarding 20°C)	
Flow velocity 0...6m/s:	max. ±1%LEL or +15% of the display @Flow velocities ≥1.5m/s			
Cross sensitivities @ 50% LEL:	<u>Gas supply</u>	<u>CH₄ display</u>	<u>C₃H₈ display</u>	<u>n hexane display</u>
	2.00Vol.% H ₂	about 65%LEL	about100%LEL	about 135%LEL(theor.)
	2.20Vol.% CH ₄	= 50%LEL	about 75%LEL	about 100%LEL
	1.15Vol.% C ₂ H ₄	about 48%LEL	about 58%LEL	about 77%LEL
	0.85Vol.% C ₃ H ₈	about 33%LEL	= 50%LEL	about 65%LEL
	0.70Vol.% C ₄ H ₁₀	about 31%LEL	about 47%LEL	about 62%LEL
	0.55Vol.% C ₅ H ₁₂	about 28%LEL	about 40%LEL	about 52%LEL
	0.50Vol.% C ₆ H ₁₄	about 27%LEL	about 38%LEL	= 50%LEL
	0.45Vol.% C ₇ H ₁₆	about 19%LEL	about 28%LEL	about 35%LEL
	0.40Vol.% C ₈ H ₁₈	about 15%LEL	about 23%LEL	about 29%LEL
	They can vary from one sensor to another and depend on the gas concentration as well as on the age of the sensor.			
Expected service life:	3 years in pure air			

MK221-1 Catalytic combustion sensor for flammable gases (with increased contamination resistance)				
Measuring ranges:	0.0...100%LEL		0.00...5.00Vol.% CH ₄	
Resolution / tolerance band:	0.5 / ±2.5%LEL		0.02 / ±0.14Vol.% CH ₄	
Setting time:	t ₅₀ ≤ 10 sec	t ₉₀ ≤ 20 sec	@ CH ₄ (methane)	
	t ₅₀ ≤ 12 sec	t ₉₀ ≤ 30 sec	@ C ₃ H ₈ (propane)	
	t ₅₀ ≤ 40 sec	t ₉₀ ≤ 105sec	@ C ₆ H ₁₄ (n hexane)	
Pressure (70)80....120(130)kPa:	max. ±5(7)%LEL or ±10% of the display		(regarding 100kPa)	
Humidity 0%...95% RH:	max. ±3%LEL or ±10% of the C ₃ H ₈ display		(regarding 0% RH @40°C)	
	or ±20% of the CH ₄ display		(regarding 0% RH @40°C)	
Temperature(-20)-10...+40(55)°C:	max. ±3%LEL or ±10(15)% of the display		(regarding 20°C)	
Flow velocity 0...6m/s:	max. ±1%LEL or +20% of the display @Flow velocities ≥1.5m/s			
Cross sensitivities @ 50% LEL:	<u>Gas supply</u>	<u>CH₄ display</u>	<u>C₃H₈ display</u>	<u>n hexane display</u>
	2.00Vol.% H ₂	about 65%LEL	about100%LEL	about 135%LEL(theor.)
	2.20Vol.% CH ₄	= 50%LEL	about 75%LEL	about 100%LEL
	1.15Vol.% C ₂ H ₄	about 48%LEL	about 58%LEL	about 77%LEL
	0.85Vol.% C ₃ H ₈	about 33%LEL	= 50%LEL	about 65%LEL
	0.70Vol.% C ₄ H ₁₀	about 30%LEL	about 47%LEL	about 62%LEL
	0.55Vol.% C ₅ H ₁₂	about 26%LEL	about 40%LEL	about 52%LEL
	0.50Vol.% C ₆ H ₁₄	about 25%LEL	about 38%LEL	= 50%LEL
	They can vary from one sensor to another and depend on the gas concentration as well as on the age of the sensor.			
Expected service life:	3 years in pure air			

MK222-0 Photoionisation sensor for toxic flammable vapours or VOCs						
		Trichlor-ethylene		MIBK	c-Hexane	
		Benzene		Acetone	Heptane	
		Toluene	MEK	Diethyl ether	Octane	
	Styrene	Xylene	Diesel	Propene	n nonane	n butanol
Measuring gases:	Kerosene			Petrol	Vinyl chloride	Ethyl acetate
Measuring ranges:	0-800ppm	0-1000ppm	0-1500ppm	Isobutylene	Methyl bromide	n hexane
Resolution (<100ppm):	0.2ppm	0.2ppm	0.5ppm	0-2000ppm	0-3000ppm	0-6000ppm
Tolerance band:	±0.5ppm	±0.6ppm	±0.9ppm	0.5ppm	0.5ppm	1ppm
Setting time:	t ₉₀ < 30sec			±1.2ppm	±1.8ppm	±3ppm
Ionization potential:	10.6 eV					
Cross sensitivities:	Kerosene: about 250%; C ₈ H ₈ :250%; C ₇ H ₈ :190%; C ₆ H ₆ :190%; Diesel:about 110%;					
(iC ₄ H ₈ =100%)	Petrol:about 90%; C ₃ H ₆ 0:83%; C ₈ H ₁₈ :45%; C ₇ H ₁₆ :40%; H ₂ S:30%; C ₆ H ₁₄ :22%;					
	NO:14%; NH ₃ :11%; C ₅ H ₁₂ :10%; C ₄ H ₁₀ :0%; C ₃ H ₈ :0%; CH ₄ :0%; H ₂ :0%;					
Response faktors RF:	1-Butanol =3.40	Cyclohexane =1.50	Heptane =2.50	n nonan =1.60		
	1-Propanol =5.70	Decane =1.60	Isobutanol =4.70	n pentane =9.70		
	Acetone =1-20	Diesel fuel 1 =0.90	Isobutylene =1.00	NO =7.20		
	Ammonia =9.40	Diesel fuel 2 =0.75	Isopropanol =5.60	Octane =2.20		
	Arsine =2,60	Diethyl ether =1.20	Jet A fuel =0.40	Phosphine =2.80		
	Petrol =1.10	Ethyl acetate =4.20	JP5 fuel =0.48	Propylene =1.30		
	Benzene =0.53	Ethyl acrylate =2.30	Methyl acetate =7.00	Styrene =0.40		
	Butadiene =0.69	Ethyl mercaptan =0.60	Methyl mercaptan =0.60	Toluene =0.53		
	Butyl acetate =2.40	H2S =3.20	n hexane =4.50	Xylene =0.50		
Expected service life:	2...3 years in pure air					
MK248-8/MK245-1 Infrared sensors for carbon dioxide CO ₂						
Measuring range:	0.02...5.00Vol.%		oder	0.00...25Vol.%		
Resolution:	0.01...0.05Vol.%		oder	0.01...0.5Vol.%		
Setting time:	t ₅₀ ≤ 20sec		t ₉₀ ≤ 50sec	t ₁₀ ≤ 50sec @ CO ₂		
Pressure	70...130kPa:	<1,6% of the display per 1% pressure change				(regarding 100kPa)
Humidity	0%...95% RH:	max. ±0.01 Vol.% or ±2% of the display				(regarding 50%RH @20°C)
Temperature	-20...+55°C:	max. ±0,02 Vol.% or ±10% of the display				(regarding 20°C)
Long term stability	per month:	max. ±0.01 Vol.% or ±2% of the display conditions)				(under laboratory
Expected service life:	6 years					
MK249-8/MK245-1 Infrared sensors for flammable gases and vapours						
Measuring range:	0,0...100%LEL		0.00...100Vol.% CH ₄			
Resolution:	0.2...1.0%LEL		0.01...0.5Vol.% CH ₄			
Tolerance band:	±1.2% LEL		±0.05Vol.% CH ₄			
Setting time:	t ₅₀ ≤ 20sec		t ₉₀ ≤ 45 sec	@ CH ₄ (methane)		
	t ₅₀ ≤ 25sec		t ₉₀ ≤ 66 sec	@ C ₃ H ₈ (propane)		
	t ₅₀ ≤ 30sec		t ₉₀ ≤ 99 sec	@ C ₆ H ₁₄ (n hexane)		
	t ₅₀ ≤ 55sec		t ₉₀ ≤ 371sec	@ C ₉ H ₂₀ (n nonane)		
Pressure	70...130kPa:	<1.5% of the CH ₄ display per 1% pressure change				(regarding 100kPa)
		<1.2% of the C ₃ H ₈ display per 1% pressure change				(regarding 100kPa)
Humidity	0%...95% RH:	max. ±2,0 %LEL or ±15% of the display				(regarding 0%RH @40°C)
Temperature	-20...+50°C:	max. ±2.0 %LEL or ±10% of the C ₃ H ₈ display				(regarding 20°C)
Cross sensitivities	@ 50%LEL:	<u>Gas supply display.</u>	<u>CH₄ display</u>	<u>C₃H₈ display</u>	<u>n hexane display</u>	<u>n nonane</u>
		0.85Vol% C ₃ H ₈	about 145%LEL	= 50%LEL	about 67%LEL	about 80%LEL
		1.20Vol% C ₂ H ₆	about 138%LEL	about 48%LEL	about 65%LEL	about 78%LEL
		0-70Vol% C ₄ H ₁₀	about 110%LEL	about 42%LEL	about 57%LEL	about 69%LEL
		1-00Vol% C ₃ H ₈ O	about 97%LEL	about 39%LEL	about 53%LEL	about 64%LEL
		0.50Vol% C ₆ H ₁₄	about 88%LEL	about 37%LEL	= 50%LEL	about 60%LEL
		0.55Vol% C ₅ H ₁₂	about 87%LEL	about 36%LEL	about 49%LEL	about 59%LEL
		0,45Vol% C ₇ H ₁₆	about 82%LEL	about 34%LEL	about 47%LEL	about 57%LEL
		1.00Vol% C ₄ H ₈ O ₂	about 69%LEL	about 31%LEL	about 41%LEL	about 50%LEL
		0.35Vol% C ₉ H ₂₀	about 65%LEL	about 31%LEL	about 41%LEL	= 50%LEL
		2.20Vol% CH ₄	= 50%LEL	about 26%LEL	about 35%LEL	about 42%LEL
		0-75Vol% C ₄ H ₈ O	about 41%LEL	about 22%LEL	about 28%LEL	about 34%LEL
		1-25Vol% C ₃ H ₆ O	about 26%LEL	about 16%LEL	about 22%LEL	about 27%LEL
		0.50Vol% C ₇ H ₈	about 26%LEL	about 16%LEL	about 22%LEL	about 26%LEL
Expected service life:	They can vary from one sensor to another and are depending on the gas concentration. 6 years					
MK349-8 Electrochemical sensor for phosgene COCl ₂ (PGN)						
Measuring range:	0...2ppm					
Resolution / tolerance band:	0.01ppm / ±0.02ppm					
Setting time:	t ₉₀ < 150sec					
Pressure	80...120kPa:	max. ±0.02ppm or ±10% of the display				(regarding 100kPa)
Humidity	10%...95% RH:	max. ±0.02ppm or ±10% of the display				(regarding 50%RH @20°C)
Temperature	-20...+40°C:	max. ±0.02ppm or ±10% of the display				(regarding 20°C)
Cross sensitivities:	ClO ₂ : -300%; HCl: 250%; AsH ₃ : 90%; Cl ₂ : 40%; NO ₂ : -10%; O ₃ : 10%; (*1)					
Expected service life:	1...1.5 years in air					

MK353-8 Electrochemical sensor for phosphine PH₃			
Measuring ranges:	0...10ppm	0...20ppm	0...50ppm
Resolution / tolerance band:	0.05ppm / ±0.05ppm	0.05ppm / ±0.05ppm	0.05ppm / ±0.05ppm
Setting time:	t ₅₀ < 20sec	t ₉₀ < 60sec	
Pressure 80...120kPa:	max. ±0.05ppm or ±10% of the display		(regarding 100kPa)
Humidity 15%...90% RH:	max. ±0.05ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+50°C:	max. ±0.05ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	SiH ₄ :90%; GeH ₄ :90%; AsH ₃ :65%; B ₂ H ₆ :35%; SO ₂ :20%; CO:0,5%; H ₂ :0.1%; (*1)		
Expected service life:	2...3 years in air		
MK379-8 Electrochemical sensor for ethylene oxide C₂H₄O (ETO)			
Measuring ranges:	0...20ppm	0...50ppm	0...100ppm
Resolution / tolerance band:	0.1ppm / ±0.3ppm	0.1ppm / ±0.3ppm	0.1ppm / ±0.3ppm
Setting time:	t ₅₀ < 30sec	t ₉₀ < 120sec	
Pressure 80...120kPa:	max. ±1ppm or ±15% of the display		(regarding 100kPa)
Humidity 15%...90% RH:	max. ±2ppm or ±15% of the display		(regarding 50%RH @20°C)
Temperature (-20)0...+40[50]°C:	max. ±1[2]ppm or ±15(20)% of the display		(regarding 20°C)
Cross sensitivities:	CO≈40%; CH ₄ O≈150%; C ₂ H ₂ ≈125%; CH ₂ O≈120%; CH ₄ S≈100%; C ₂ H ₄ ≈80%; C ₂ H ₆ O≈55%; C ₄ H ₁₀ O≈40%; C ₇ H ₈ ≈20%; MEK≈10%; among others		
Expected service life:	2...3 years in air		
Running-in time:	4 minutes up to 7 days – depending on the interruption time		
MK380-8 Electrochemical sensor for carbon monoxide CO and hydrogen sulphide H₂S (COSH)			
Measuring ranges:	0...500ppm CO (at EC0)	0...100ppm H ₂ S (at EC1)	
Resolution / tolerance band:	1ppm / ±3ppm CO	0.2ppm / ±0.6ppm H ₂ S	
Setting time:	t ₅₀ < 20sec	t ₉₀ < 50sec	
Pressure 80...120kPa:	max. ±3(1)ppm or ±7(10)% of the CO (H ₂ S) display		(regarding 100kPa)
Humidity 15%...90% RH:	max. ±3(1)ppm or ±7(10)% of the CO (H ₂ S) display		(regarding 50%RH @20°C)
Temperature -20...+50°C:	max. ±3(1)ppm or ±15(10)% of the CO (H ₂ S) display		(regarding 20°C)
Cross sensitivities CO display:	H ₂ S:0...40%; H ₂ ≈20%; SO ₂ <20%; NO ₂ <2%; NO<0.3%; Cl ₂ :0%; (*1)		
Cross sensitivities H ₂ S display:	CO<2%; NO ₂ ≈-20%; SO ₂ :8...20%; NO<3%; H ₂ :0.03%; Cl ₂ :0%; (*1)		
Expected service life:	3 years in air		
MK383-8 Electrochemical sensor for oxygen O₂			
Measuring range:	0...25Vol. %		
Resolution / tolerance band:	0,1Vol. % / ±0,3Vol. %		
Setting time:	t ₂₀ ≤ 6sec	t ₉₀ ≤ 20sec	
Pressure 80...120kPa:	max. ±0.2Vol. % or ±2.5% of the measuring range		(regarding 100kPa)
Humidity 0%...90% RH:	max. ±0.2Vol. % or ±2.5% of the measuring range		(regarding 50%RH @40°C)
Temperature -20...+50°C:	max. ±0.5Vol. % or ±2.5% of the display		(regarding 20°C)
Expected service life:	2 years in air		
MK390-8 Electrochemical sensor for chorine Cl₂			
Measuring ranges:	0...10ppm	0...20ppm	0...40ppm
Resolution / tolerance band:	0.05ppm / ±0.10ppm	0.05ppm / ±0.10ppm	0.1ppm / ±0.1ppm
Setting time:	t ₅₀ < 10sec	t ₉₀ < 30sec	
Pressure 80...120kPa:	max. ±0.2ppm or ±10% of the display		(regarding 100kPa)
Humidity 10%...95% RH:	max. ±0.2ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+50°C:	max. ±0.2ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	ClO ₂ :50%; F ₂ :40%; NO ₂ :20%; O ₃ :20%; SO ₂ :18%; CO ₂ :0%; CO:0%; H ₂ S:0%; H ₂ :0% (*1)		
Expected service life:	2...3 years in air		
MK391-8 Electrochemical sensor for chlorine dioxide ClO₂ (CLO)			
Measuring range:	0...2ppm		
Resolution / tolerance band:	0.01ppm / ±0.03ppm		
Setting time:	t ₉₀ < 120sec		
Pressure 80...120kPa:	max. ±0.05ppm or ±10% of the display		(regarding 100kPa)
Humidity 10%...95% RH:	max. ±0.05ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+50°C:	max. ±0.05ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	Cl ₂ ≈60%; O ₃ :-280%; H ₂ S:-25%; H ₂ : 0%; CO: 0%; (*1)		
Expected service life:	1...2 years in air		
MK392-8 Electrochemical sensor for hydrogen chlorine HCl			
Measuring ranges:	0...30ppm	0...50ppm	
Resolution / tolerance band:	0.2ppm / ±0.4ppm	0.2ppm / ±0.4ppm	
Setting time:	t ₅₀ < 30sec	t ₉₀ < 90sec	
Pressure 80...120kPa:	max. ±1ppm or ±10% of the display		(regarding 100kPa)
Humidity 10%...95% RH:	max. ±1ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+50°C:	max. ±1ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	AsH ₃ :350%; PH ₃ :300%; H ₂ S:65%; NO:45%; SO ₂ :40%; HCN:35%; Cl ₂ :6%; NO ₂ :3%; NH ₃ :0.1%; CO:0%; CO ₂ :0%; H ₂ :0%; (*1)		
Expected service life:	2...3 years in air		

MK396-8 Electrochemical sensor for hydrogen H₂ (*2)				
Measuring range:	0...2000ppm			
Resolution / tolerance band:	2ppm / ±50ppm			
Setting time:	t ₅₀ < 30sec t ₉₀ < 90sec			
Pressure	80...120kPa:	max. ±10ppm or ±10% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±10ppm or ±10% of the display		(regarding 50%RH)
Temperature	-20...+50°C:	max. ±20ppm or ±20% of the display		(regarding 20°C)
Cross sensitivities:	C ₂ H ₄ ≈80%; NO≈35%; HCN≈30%; CO<20%; H ₂ S<20%; NO ₂ =SO ₂ =Cl ₂ =HCl=0%; (*1)			
Expected service life:	2...3 years in air			
MK402-8 Electrochemical sensor for hydrogen H₂ (*2)				
Measuring range:	0...1.00Vol.%			
Resolution / tolerance band:	0.01Vol.% / ±0.02Vol.%			
Setting time:	t ₅₀ < 40sec t ₉₀ < 70sec			
Pressure	80...120kPa:	max. ±0.01Vol.% or ±10% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±0.01Vol.% or ±10% of the display		(regarding 50%RH)
Temperature	-20...+50°C:	max. ±0,02Vol.% or ±20% of the display		(regarding 20°C)
Cross sensitivities:	NO ₂ :~400%; CO:150%; H ₂ S:20%; C ₂ H ₄ :yes; NH ₃ =CO ₂ =Cl ₂ =SO ₂ =HCN=0%; (*1)			
Expected service life:	2...3 years in air			
MK403-8 Electrochemical sensor for hydrogen H₂ (*2)				
Measuring range:	0...4.00Vol.%			
Resolution / tolerance band:	0.01Vol.% / ±0.05Vol.%			
Setting time:	t ₅₀ < 40sec t ₉₀ < 60sec			
Pressure	80...120kPa:	max. ±0.01Vol.% or ±10% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±0.01Vol.% or ±10% of the display		(regarding 50%RH)
Temperature	-20...+50°C:	max. ±0.02Vol.% or ±25% of the display		(regarding 20°C)
Cross sensitivities:	H ₂ S:220%; C ₂ H ₄ :yes; NH ₃ =CO ₂ =CO=Cl ₂ =HCN=NO=NO ₂ =0%; (*1)			
Expected service life:	2...3 years in air			
MK409-8 Electrochemical sensor for hydrogen cyanide HCN				
Measuring ranges:	0...50ppm	0...100ppm		
Resolution / tolerance band:	0.1ppm / ±0.5ppm	0.2ppm / ±1.0ppm		
Setting time:	t ₅₀ < 25sec t ₉₀ < 60sec			
Pressure	80...120kPa:	max. ±0.5ppm or ±10% of the display		(concerning 100kPa)
Humidity	10%...95% RH:	max. ±0.5ppm or ±10% of the display @20°C)		(concerning 50% RH
Temperature	-20...+50°C:	max. ±0.5ppm or ±15% of the display		(concerning 20°C)
Cross sensitivities:	NO ₂ ≈70%, NO≈5%, H ₂ S≈0...200% (depending on the filter saturation) CO=CO ₂ =H ₂ =0% (*1)			
Expected service life:	2 years in air			
MK412-3/MK412-9 Electrochemical sensors for hydrogen fluoride HF				
Measuring ranges:	0...10ppm	0...10ppm		
Resolution / tolerance band:	0.1ppm / ±0.3ppm (MK412-3)	0.5ppm / ±0.5ppm (MK412-9)		
Setting time:	t ₅₀ < 40sec t ₉₀ < 90sec			
Pressure	80...120kPa:	max. ±0,2ppm or ±10% of the display		(regarding 100kPa)
Humidity	10%...80% RH:	max. ±0.2ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature	-20...+40°C:	max. ±0.2ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	HCl:66%; Cl ₂ :40%; CO=CO ₂ =NO ₂ =H ₂ S=H ₂ =0% (*1)			
Expected service life:	1..2 years in air			
MK427-8 Electrochemical sensor for oxygen O₂				
Measuring range:	0...25Vol.%			
Resolution / tolerance band:	0.1Vol.% / ±0,3Vol.%			
Setting time:	t ₂₀ ≤ 8sec t ₉₀ ≤ 25sec			
Pressure	(70)80...120(130)kPa:	max. ±0.4(0.6)Vol.% or ±2(3)% of the measuring range		(regarding 100kPa)
Humidity	0%...95% RH:	max. ±0.5Vol.% or ±2.5% of the measuring range		(regarding 50%RH @40°C)
Temperature	(-20)-10...+55°C:	max. ±0.5(0.8)Vol.% or ±2.5(4.0)% of the display		(regarding 20°C)
Expected service life:	3 years in air			
MK440-8 Electrochemical sensor for sulphur dioxide SO₂				
Measuring ranges:	0...10ppm	0...20ppm	0...50ppm	0...100ppm
Resolution:	0.05ppm	0.05ppm	0.1ppm	0.1ppm
Tolerance band:	±0.15ppm	±0.20ppm	±0.3ppm	±0.4ppm
Setting time:	t ₅₀ < 10sec t ₉₀ < 30sec			
Pressure	80...120kPa:	max. ±0.2ppm or ±5% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±0.3ppm or ±3% of the display		(regarding 50%RH @20°C)
Temperature	-20...+50°C:	max. ±0,3ppm or ±5% of the display		(regarding 20°C)
Cross sensitivities:	C ₂ H ₂ <300%; NO ₂ <-170%; C ₂ H ₄ <90%; HCN<50%; Cl ₂ <-40%; NO<10%; H ₂ S<0,4%; CO<0,4%; H ₂ <0,3%; NH ₃ =0%; (*1)			
Expected service life:	3 years in air			

MK443-8 Electrochemical sensor for carbon monoxide CO				
Measuring ranges:	3...500ppm	3...1000ppm	3...2000ppm	
Resolution / tolerance band:	1ppm / ±3ppm	1ppm / ±3ppm	1ppm / ±3ppm	
Setting time:	t ₅₀ < 10sec	t ₉₀ ≤ 30sec	t ₁₀ < 30sec (decay time)	
Pressure	80...120kPa:	max. ±3ppm or ±10% of the display		(regarding 100kPa)
Humidity	15%...95% RH:	max. ±3ppm or ±5% of the display		(regarding 50%RH @20°C)
Temperature	-20...+40(55)°C:	max. ±3ppm or ±5(10)% of the display		(regarding 20°C)
Cross sensitivities:	C ₂ H ₄ ≈96%, C ₂ H ₂ ≈90%, H ₂ <30%(typ.15%), NO<20%, Cl ₂ <7%, C ₂ H ₆ O□0.5%, SO ₂ =NH ₃ =H ₂ S=0% (*1)			
Expected service life:	3 years in air			
MK445-8 Electrochemical sensor for hydrogen sulphide H₂S				
Measuring ranges:	0.2...50ppm	0.2...100ppm	0.2...200ppm	0.5...500ppm
Resolution:	0.1ppm	0.1ppm	0.2ppm	0.5ppm
Tolerance band:	±0.5ppm	±0.5ppm	±1.0ppm	±1.5ppm
Setting time:	t ₅₀ < 10sec	t ₉₀ < 30sec	t ₁₀ < 30sec (decay time)	
Pressure	80...120kPa:	max. ±0.2ppm or ±5% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±0.2ppm or ±5% of the display		(regarding 50%RH @20°C)
Temperature	-20...+40(55)°C:	max. ±0.2ppm or ±5(10)% of the display		(regarding 20°C)
Cross sensitivities:	NO ₂ <10%, CO<2%, NO<1%, CO ₂ =SO ₂ =Cl ₂ =NH ₃ =C ₂ H ₄ =0% little Methanol cross sensitivity (*1)			
Expected service life:	3 years in air			
MK453-8 Electrochemical sensor for ammonia NH₃				
Measuring ranges:	0...300ppm	0...500ppm		
Resolution / tolerance band:	1ppm / ±3ppm	1ppm / ±3ppm		
Setting time:	t ₉₀ < 45sec			
Pressure	80...120kPa:	max. ±1ppm or ±10% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±1ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature	-(20)10...+50°C:	max. ±1(2)ppm or ±15(20)% of the display		(regarding 20°C)
Cross sensitivities:	H ₂ S≈120%, NO ₂ ≈100%, SO ₂ ≈30%, CO=NO=CO ₂ =H ₂ =C ₂ H ₆ O=0% (*1)			
Expected service life:	2..3 years in pure air			
MK454-8 Electrochemical sensor for ammonia NH₃				
Measuring ranges:	0...500ppm	0...1000ppm	0...1500ppm	
Resolution / tolerance band:	2ppm / ±5ppm	5ppm / ±10ppm	5ppm / ±10ppm	
Setting time:	t ₉₀ < 60sec		(at 20°C)	
Pressure	80...120kPa:	max. ±5ppm or ±10% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±5ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature	-20...+55°C:	max. ±10ppm or ±20% of the display		(regarding 20°C)
Cross sensitivities:	H ₂ S≈140%, NO ₂ ≈100%, SO ₂ ≈30%, CO=NO=CO ₂ =H ₂ =C ₂ H ₆ O=0% (*1)			
Expected service life:	2..3 years in pure air			
MK457-8 Electrochemical sensor for nitrogen monoxide NO				
Measuring ranges:	0...50ppm	0...100ppm	0...200ppm	
Resolution / tolerance band:	0.2ppm / ±1.5ppm	0.5ppm / ±2.0ppm	0.5ppm / ±2.0ppm	
Setting time:	t ₅₀ < 15sec	t ₉₀ < 45sec	(at 20°C)	
Pressure	80...120kPa:	max. ±1ppm or ±10% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±1ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature	-20...+40(50)°C:	max. ±2ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	H ₂ S<50%; NO ₂ <40%; C ₂ H ₆ O ±10%; SO ₂ <5%; H ₂ <1%; NH ₃ <1%; CO<-1%; CO ₂ =CL ₂ =0; (*1)			
Expected service life:	3 years in air			
Running-in time:	3 minutes to 1 day – depending on the interruption time			
MK458-8 Electrochemical sensor for nitrogen dioxide NO₂				
Measuring ranges:	0...30ppm	0...50ppm	0...100ppm	
Resolution / tolerance band:	0.1ppm / ±0.3ppm	0.1ppm / ±0.5ppm	0.1ppm / ±0.5ppm	
Setting time:	t ₅₀ < 10sec	t ₉₀ < 30sec	(at 20°C)	
Pressure	80...120kPa:	max. ±0,2ppm or ±10% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±0,2ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature	-20...+50°C:	max. ±0,2ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	Cl ₂ ≈100%; H ₂ S<-40%; NO<20%; C ₂ H ₆ O<1%; CO<-1%; SO ₂ <-1%; H ₂ <-1%; NH ₃ <-1%, CO ₂ =0; (*1)			
Expected service life:	3 years in air			
MK460-8 Electrochemical sensor for silane SiH₄				
Measuring ranges:	0...20ppm	0...50ppm		
Resolution / tolerance band:	0.1ppm / ±0.2ppm	0.1ppm / ±0.2ppm		
Setting time:	t ₅₀ < 20sec	t ₉₀ < 60sec		
Pressure	80...120kPa:	max. ±0,1ppm or ±10% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±0,2ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature	-20...+50°C:	max. ±0.3ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	H ₂ S≈160%, PH ₃ ≈100%; SO ₂ ≈20%; H ₂ =CO=0%; (*1)			
Expected service life:	2..3 years in air			

For (*1): Gas display regarding the supplied concentration in the range of AGW (MAK) values

For (*2): Not permitted for the monitoring of the lower explosion limit for applications of the primary explosion protection

3.11 Alarm limit values - Basic setting

Basic setting of the alarm thresholds for toxic gases without exposure alert

Measuring range	Alarm 1	Alarm 2	STEL (15')	TWA (8h)
0 ... 20ppm C ₂ H ₄ O (ETO)	2.0ppm	4.0ppm	-	-
0 ... 2000ppm C ₄ H ₈	100ppm	200ppm	-	-
0 ... 10ppm Cl ₂	0.5ppm	1.0ppm	-	-
0 ... 2ppm ClO ₂ (CLO)	0.2ppm (*1)	0.4ppm	-	-
0 ... 2ppm COCl ₂ (PGN)	0.1ppm	0.2ppm	-	-
0 ... 500ppm CO	30ppm	60ppm	-	-
0 ... 5.0Vol.% CO ₂	0.5Vol. %	1.0Vol. %	-	-
0 ... 100ppm H ₂ S	5.0ppm	10ppm	-	-
0 ... 30ppm HCl	5.0ppm (*1)	10ppm	-	-
0 ... 50ppm HCN	5.0ppm (*1)	10ppm	-	-
0 ... 10ppm HF	1.0ppm	2.0ppm	-	-
0 ... 300ppm NH ₃	20ppm	40ppm	-	-
0 ... 100ppm NO	2.5ppm (*1)	5.0ppm	-	-
0 ... 30ppm NO ₂	2.0ppm (*1)	4.0ppm	-	-
0 ... 10ppm PH ₃	0.3ppm (*1)	0.6ppm	-	-
0 ... 20ppm SiH ₄ (SIL)	5.0ppm	10ppm	-	-
0 ... 10ppm SO ₂	1.0ppm	2.0ppm	-	-

For (*1): A monitoring of the AGW value is not satisfactory possible with the available sensor technology.

Basic setting of the alarm thresholds for toxic gases with exposure alert

Measuring range	Alarm 1	Alarm 2	STEL (15')	TWA (8h)
0 ... 20ppm C ₂ H ₄ O	2ppm	6ppm	4ppm	2ppm
0 ... 2000ppm C ₄ H ₈	100ppm	400ppm	200ppm	100ppm
0 ... 10ppm Cl ₂	1.0ppm	1.5ppm	1.0ppm	0.5ppm
0 ... 2ppm ClO ₂	0.2ppm	0.4ppm	0.2ppm	0.1ppm
0 ... 2ppm COCl ₂	0.1ppm	0.2ppm	0.2ppm	0.1ppm
0 ... 500ppm CO	30ppm	120ppm	60ppm	30ppm
0 ... 5.0Vol.% CO ₂	0.5Vol. %	2.0Vol. %	1.0Vol. %	0.5Vol. %
0 ... 100ppm H ₂ S	5.0ppm	15ppm	10ppm	5.0ppm
0 ... 30ppm HCl	5.0ppm	10ppm	5.0ppm	2.0ppm
0 ... 50ppm HCN	5.0ppm	10ppm	5.0ppm	1.9ppm
0 ... 10ppm HF	1.0ppm	3.0ppm	2.0ppm	1.0ppm
0 ... 300ppm NH ₃	20ppm	80ppm	40ppm	20ppm
0 ... 100ppm NO	2.5ppm	5.0ppm	2.5ppm	0.5ppm
0 ... 30ppm NO ₂	2.0ppm	4.0ppm	2.0ppm	0.5ppm
0 ... 10ppm PH ₃	0.3ppm (*1)	0.4ppm	0.2ppm	0.1ppm
0 ... 20ppm SiH ₄	5.0ppm	15ppm	10ppm	5.0ppm
0 ... 10ppm SO ₂	1.0ppm	3.0ppm	2.0ppm	1.0ppm

For (*1): A monitoring of the AGW value is not satisfactory possible with the available sensor technology.

Basic setting of the alarm thresholds for oxygen and for flammable gases and vapours

Measuring range	Alarm 1	Alarm 2	Alarm 3
0 ... 25Vol.% O ₂	19.0Vol. % (↓)	17.0Vol. (↓)	23.0Vol. % (↑)
0 ... 2000ppm H ₂ (*2)	1000ppm	1500ppm	2000ppm
0 ... 1.0/4.0Vol.% H ₂ (*2)	0.40Vol. %	0.60Vol. %	0.80Vol. %
0 ... 5.0Vol.% CH ₄	1.00Vol. %	2.00Vol. %	3.00Vol. %
0 ... 100%LEL CH ₄ (*3)	20.0%LEL	40.0%LEL	60.0%LEL

For (*2): Not permitted for the monitoring of the lower explosion limit for applications of the primary explosion protection.

For (*3): or another of the following listed flammable gases and vapours

LEL values according to the DIN EN 60079-20-1:2010					
4.0Vol.% H ₂	hydrogen	(CAS-No.1333-74-0)	6.0Vol.% CH ₄ O	methanol	(CAS-No.67-56-1)
4.4Vol.% CH ₄	methane	(CAS-No.74-82-8)	3.1Vol.% C ₂ H ₆ O	ethanol	(CAS-No.64-17-5)
2.3Vol.% C ₂ H ₂	acetylene	(CAS-No.74-86-2)	2.5Vol.% C ₃ H ₆ O	acetone	(CAS-No.67-64-1)
2.3Vol.% C ₂ H ₄	ethylene	(CAS-No.74-85-1)	3.1Vol.% C ₃ H ₆ O ₂	methyl acetate	(CAS-No.79-20-9)
2.4Vol.% C ₂ H ₆	ethane	(CAS-No.74-84-0)	2.7Vol.% C ₃ H ₆ O ₂	ethyl formate ETF	(CAS-No.109-94-4)
1.7Vol.% C ₃ H ₈	propane	(CAS-No.74-98-6)	2.0Vol.% C ₃ H ₈ O	isopropyl	(CAS-No.67-63-0)
1.4Vol.% C ₄ H ₁₀	butane	(CAS-No.106-97-8)	1.5Vol.% C ₄ H ₈ O	methyl ethyl ketone MEK	(CAS-No.78-93-3)
1.1Vol.% C ₅ H ₁₂	pentane	(CAS-No.109-66-0)	2.0Vol.% C ₄ H ₈ O ₂	ethyl acetate	(CAS-No.141-78-6)
1.0Vol.% C ₆ H ₁₄	n-hexane	(CAS-No.110-54-3)	1.4Vol.% C ₄ H ₁₀ O	n-butanol	(CAS-No.71-36-3)
0.85Vol.% C ₇ H ₁₆	heptane	(CAS-No.142-82-5)	1,2Vol.% C ₆ H ₁₂ O	Methyl isobutyl ketone MIBK	(CAS-Nr.108-10-1)
0.70Vol.% C ₉ H ₂₀	n-nonane	(CAS-No.111-84-2)	1.0Vol.% C ₇ H ₈	toluene	(CAS-No.108-88-3)

3.12 Technical data

Type designations:	G999C (with slot for a catalytic combustion sensor CC) G999E (with slot for a fourth electrochemical sensor EC) G999P (with slot for a photoionisation sensor PID)																												
Measuring principle:	Electrochemical (EC): For toxic gases and oxygen Photoionisation (PID): For toxic flammable gases and vapours Catalytic combustion (CC): For flammable gases and vapours (up to 100%LEL)For Infrared (IR): flammable gases and vapours and carbon dioxide																												
Measuring ranges:	Refer to the chapter “Sensor types and measuring ranges” and “Sensor specification”																												
Setting time:	Refer to the chapter “Sensor specification”																												
Sensor service life:	Refer to the chapter “Sensor specification”																												
Measuring gas supply:	Via the diffusion opening while the pump is switched off or via the suction opening during the pump operation (sensor cover closed)																												
Pump capacity:	0,5...0,6slpm @0kPa / 0,30slpm @-4kPa / 0,0slpm@-12kPa max.100m hose length (depending on the measuring gas and hose)																												
Display:	Illuminated LCD full graphics display, automatic size setting for optimum reading, display of the battery capacity, gas concentration as current value and peak value																												
Alerting:	Depending on the gas type 3 or 2 instantaneous value and 2 exposure level alarms, battery alarm with visual and acoustical signalling as well as display on the screen, colour of the display depending on the alarm state (orange/red) Horn: 103 dB(A) (can be reduced to 90 dB(A))																												
Zero point and sensitivity adjustment:	Manual or automatic with an adjustment program, if necessary, test gas supply via the “SMART CAP” with 0.5...0.6slpm																												
Radio:	optionally 868MHz for Europe; Range about 700m (free field) optionally 915MHz for US; Range about 300m (free field)																												
Power supply:	5.2V 2100mAh NiMH battery module; rechargeable																												
Service life (*1)	<table><tr><td rowspan="4">Without radio:</td><td>about 26h (EC+CC_{CH4}+IR)</td><td>about 18h (EC+CC+IR)</td><td>about 11h (EC+CC+IR+Pmp)</td></tr><tr><td>about 42h (EC+CC_{CH4})</td><td>about 25h (EC+CC)</td><td>about 13h (EC+CC+Pump)</td></tr><tr><td>about 52h (EC+PID)</td><td>about 30h (EC+PID+IR)</td><td>about 14h (EC+PID+IR+Pmp)</td></tr><tr><td>about 130h (EC)</td><td>about 47h (EC+IR)</td><td>about 17h (EC+IR+Pmp)</td></tr><tr><td rowspan="4">With radio:</td><td>about 20h (EC+CC_{CH4}+IR)</td><td>about 15h (EC+CC+IR)</td><td>about 10h (EC+CC+IR+Pmp)</td></tr><tr><td>about 28h (EC+CC_{CH4})</td><td>about 19h (EC+CC)</td><td>about 11h (EC+CC+Pmp)</td></tr><tr><td>about 33h (EC+PID)</td><td>about 22h (EC+PID+IR)</td><td>about 12h (EC+PID+IR+Pmp)</td></tr><tr><td>about 52h (EC)</td><td>about 30h (EC+IR)</td><td>about 14h (EC+IR+Pmp)</td></tr></table>	Without radio:	about 26h (EC+CC _{CH4} +IR)	about 18h (EC+CC+IR)	about 11h (EC+CC+IR+Pmp)	about 42h (EC+CC _{CH4})	about 25h (EC+CC)	about 13h (EC+CC+Pump)	about 52h (EC+PID)	about 30h (EC+PID+IR)	about 14h (EC+PID+IR+Pmp)	about 130h (EC)	about 47h (EC+IR)	about 17h (EC+IR+Pmp)	With radio:	about 20h (EC+CC _{CH4} +IR)	about 15h (EC+CC+IR)	about 10h (EC+CC+IR+Pmp)	about 28h (EC+CC _{CH4})	about 19h (EC+CC)	about 11h (EC+CC+Pmp)	about 33h (EC+PID)	about 22h (EC+PID+IR)	about 12h (EC+PID+IR+Pmp)	about 52h (EC)	about 30h (EC+IR)	about 14h (EC+IR+Pmp)		
Without radio:	about 26h (EC+CC _{CH4} +IR)		about 18h (EC+CC+IR)	about 11h (EC+CC+IR+Pmp)																									
	about 42h (EC+CC _{CH4})		about 25h (EC+CC)	about 13h (EC+CC+Pump)																									
	about 52h (EC+PID)		about 30h (EC+PID+IR)	about 14h (EC+PID+IR+Pmp)																									
	about 130h (EC)	about 47h (EC+IR)	about 17h (EC+IR+Pmp)																										
With radio:	about 20h (EC+CC _{CH4} +IR)	about 15h (EC+CC+IR)	about 10h (EC+CC+IR+Pmp)																										
	about 28h (EC+CC _{CH4})	about 19h (EC+CC)	about 11h (EC+CC+Pmp)																										
	about 33h (EC+PID)	about 22h (EC+PID+IR)	about 12h (EC+PID+IR+Pmp)																										
	about 52h (EC)	about 30h (EC+IR)	about 14h (EC+IR+Pmp)																										
Climatic conditions	<table><tr><td>For operation:</td><td>-20...+50°C</td><td> </td><td>5...95%RH</td><td> </td><td>70...130kPa</td></tr><tr><td>For storage:</td><td>-25...+55°C</td><td> </td><td>5...95%RH</td><td> </td><td>70...130kPa (recommended 0...+30°C)</td></tr></table>	For operation:	-20...+50°C		5...95%RH		70...130kPa	For storage:	-25...+55°C		5...95%RH		70...130kPa (recommended 0...+30°C)																
For operation:	-20...+50°C		5...95%RH		70...130kPa																								
For storage:	-25...+55°C		5...95%RH		70...130kPa (recommended 0...+30°C)																								
Housing	<table><tr><td>Material:</td><td>Rubberised polycarbonate</td></tr><tr><td>Dimensions:</td><td>68 x 136 x 38 mm (W x H x D)</td></tr><tr><td>Weight:</td><td>up to 370g (deviating depending on the sensor equipment)</td></tr><tr><td>Protection class:</td><td>IP67</td></tr></table>	Material:	Rubberised polycarbonate	Dimensions:	68 x 136 x 38 mm (W x H x D)	Weight:	up to 370g (deviating depending on the sensor equipment)	Protection class:	IP67																				
Material:	Rubberised polycarbonate																												
Dimensions:	68 x 136 x 38 mm (W x H x D)																												
Weight:	up to 370g (deviating depending on the sensor equipment)																												
Protection class:	IP67																												
Approvals / Tests	<table><tr><td>Markings and Ignition protection type:</td><td>G999C Ⓜ I M2 Ex ia db I Mb</td><td>Ⓜ II 2G Ex ia db IIC T4 Gb</td><td>-20°C≤Ta≤+50°C</td></tr><tr><td></td><td>G999E Ⓜ I M1 Ex ia I Ma</td><td>Ⓜ II 1G Ex ia IIC T4 Ga</td><td>-20°C≤Ta≤+50°C</td></tr><tr><td></td><td>G999P Ⓜ I M1 Ex ia I Ma</td><td>Ⓜ II 1G Ex ia IIC T4 Ga</td><td>-20°C≤Ta≤+50°C</td></tr><tr><td>EU Type examination certificate:</td><td colspan="3">BVS 15 ATEX E 064 X</td></tr><tr><td>IECEx Certificate of Conformity:</td><td colspan="3">IECEx BVS 15.0056 X</td></tr><tr><td>Electromagnetic Compatibility:</td><td>DIN EN 50270:2015</td><td>Emitted interference:</td><td>Type class I</td></tr><tr><td></td><td></td><td>Interference resistance:</td><td>Type class II</td></tr></table>	Markings and Ignition protection type:	G999C Ⓜ I M2 Ex ia db I Mb	Ⓜ II 2G Ex ia db IIC T4 Gb	-20°C≤Ta≤+50°C		G999E Ⓜ I M1 Ex ia I Ma	Ⓜ II 1G Ex ia IIC T4 Ga	-20°C≤Ta≤+50°C		G999P Ⓜ I M1 Ex ia I Ma	Ⓜ II 1G Ex ia IIC T4 Ga	-20°C≤Ta≤+50°C	EU Type examination certificate:	BVS 15 ATEX E 064 X			IECEx Certificate of Conformity:	IECEx BVS 15.0056 X			Electromagnetic Compatibility:	DIN EN 50270:2015	Emitted interference:	Type class I			Interference resistance:	Type class II
Markings and Ignition protection type:	G999C Ⓜ I M2 Ex ia db I Mb	Ⓜ II 2G Ex ia db IIC T4 Gb	-20°C≤Ta≤+50°C																										
	G999E Ⓜ I M1 Ex ia I Ma	Ⓜ II 1G Ex ia IIC T4 Ga	-20°C≤Ta≤+50°C																										
	G999P Ⓜ I M1 Ex ia I Ma	Ⓜ II 1G Ex ia IIC T4 Ga	-20°C≤Ta≤+50°C																										
EU Type examination certificate:	BVS 15 ATEX E 064 X																												
IECEx Certificate of Conformity:	IECEx BVS 15.0056 X																												
Electromagnetic Compatibility:	DIN EN 50270:2015	Emitted interference:	Type class I																										
		Interference resistance:	Type class II																										

For (*1): The service life is indicated for new battery modules at operating temperatures of +20°C. It will be reduced by pressing buttons (display lighting & lamp), by using the pump and by gas alarms. It is reduced with the age of the battery module, with the number of the charging / discharging cycles, by longer storage of the gas measurement device in the charging tray and the lazy battery effect. CC_{CH4}=with energy saving mode at a measuring range from 0-100%LEL CH₄

GfG Gesellschaft für Gerätebau mbH

Klönnestraße 99 – D-44143 Dortmund

Phone: +49 (0)231 – 564 00-0

Fax: +49 (0)231 – 51 63 13

Internet: www.gfg.biz

E-Mail: info@gfg-mbh.com



Firmware Version 1.45

215-100.30_OM_G999.doc

Dated: January, 31th, 2018

Subject to change without notice

3.13 EU-Type Examination Certificate

13	Appendix																														
14	EU-Type Examination Certificate BVS 15 ATEX E 064 X Supplement 3																														
15	Product description																														
15.1	<p>Subject and type</p> <p>The Gas detector is modified according to the descriptive documents as mentioned in the pertinent test and assessment report and receives then the marking:</p> <table border="1"> <tr> <td>Gas detector type G888C</td> <td>Marking:</td> <td>II 2G Ex ia db IIC T4 Gb</td> <td>I M2 Ex ia db I Mb</td> </tr> <tr> <td>Gas detector type G888S</td> <td>Marking:</td> <td>II 2G Ex ia db IIC T4 Gb</td> <td>I M1 Ex ia I Ma</td> </tr> <tr> <td>Gas detector type G999C</td> <td>Marking:</td> <td>II 2G Ex ia db IIC T4 Gb</td> <td>I M2 Ex ia db I Mb</td> </tr> <tr> <td>Gas detector type G999S</td> <td>Marking:</td> <td>II 2G Ex ia db IIC T4 Gb</td> <td>I M2 Ex ia db I Mb</td> </tr> <tr> <td>Gas detector type G999E</td> <td>Marking:</td> <td>II 1G Ex ia IIC T4 Ga</td> <td>I M1 Ex ia I Ma</td> </tr> <tr> <td>Gas detector type G999P</td> <td>Marking:</td> <td>II 1G Ex ia IIC T4 Ga</td> <td>I M1 Ex ia I Ma</td> </tr> </table> <p>Description</p> <p>Reason for the supplement:</p> <p>The Gas detector type G888 was renamed to type G888C (No technical changes)</p> <p>The Gas detector type G889 was renamed to type G888S (No technical changes)</p> <p>The Gas detector type G999 was renamed to type G999C (The electronic circuit was slightly modified)</p> <p>The Gas detector type G999S was renamed to type G999S (The electronic circuit was slightly modified)</p> <p>The Gas detectors type G999E and type G999P were added</p> <p>The standard EN 50303:2000 is no longer applied. The EPL Ma requirements for the Gas detector are complied by the standards listed on page 1.</p> <p>Description of Product:</p> <p>The Gas detector type G888C, type G888S, type G999C, type G999S, type G999E or type G999P is a portable instrument with a built-in power-supply battery. It is used for the detection of gases in ambient air under atmospheric conditions.</p> <p>The Gas detector type G888C, type G888S, type G999C or type G999S contains 3 electro-chemical cells, 1 IR-sensor and 1 sensor of Flameproof Enclosure</p> <p>The Gas detector type G999E contains 4 electro-chemical cells and 1 IR-sensor</p> <p>The Gas detector type G999P contains 3 electro-chemical cells, 1 IR-sensor and 1 PID-sensor</p> <p>The measurement values are shown on a built-in display. If the present limits are reached, a visual alarm, an audible alarm and a vibrating alarm are produced</p> <p>A radio module for wireless data transfer can be optionally used inside of the Gas detector type G888C, type G888S, type G999C, type G999S, type G999E or type G999P</p> <p>The gas detector type G888C, type G888S, type G999C, type G999S, type G999E or type G999P is powered by a NiMH battery which has to be charged only outside of the hazardous area.</p> <p>The gas detector type G999C, type G999S, type G999E or type G999P contains additionally a built-in pump.</p> <p>Listing of all components used referring to older standards (optionally used in type G888C, G999C, G999S)</p> <table border="1"> <tr> <th>Subject and type</th> <th>Certificate</th> <th>Standards</th> </tr> <tr> <td>Gas Sensor type A</td> <td>Sira 07ATEX1088X</td> <td>EN 60079-0:2006 EN 60079-1:2004</td> </tr> </table>	Gas detector type G888C	Marking:	II 2G Ex ia db IIC T4 Gb	I M2 Ex ia db I Mb	Gas detector type G888S	Marking:	II 2G Ex ia db IIC T4 Gb	I M1 Ex ia I Ma	Gas detector type G999C	Marking:	II 2G Ex ia db IIC T4 Gb	I M2 Ex ia db I Mb	Gas detector type G999S	Marking:	II 2G Ex ia db IIC T4 Gb	I M2 Ex ia db I Mb	Gas detector type G999E	Marking:	II 1G Ex ia IIC T4 Ga	I M1 Ex ia I Ma	Gas detector type G999P	Marking:	II 1G Ex ia IIC T4 Ga	I M1 Ex ia I Ma	Subject and type	Certificate	Standards	Gas Sensor type A	Sira 07ATEX1088X	EN 60079-0:2006 EN 60079-1:2004
Gas detector type G888C	Marking:	II 2G Ex ia db IIC T4 Gb	I M2 Ex ia db I Mb																												
Gas detector type G888S	Marking:	II 2G Ex ia db IIC T4 Gb	I M1 Ex ia I Ma																												
Gas detector type G999C	Marking:	II 2G Ex ia db IIC T4 Gb	I M2 Ex ia db I Mb																												
Gas detector type G999S	Marking:	II 2G Ex ia db IIC T4 Gb	I M2 Ex ia db I Mb																												
Gas detector type G999E	Marking:	II 1G Ex ia IIC T4 Ga	I M1 Ex ia I Ma																												
Gas detector type G999P	Marking:	II 1G Ex ia IIC T4 Ga	I M1 Ex ia I Ma																												
Subject and type	Certificate	Standards																													
Gas Sensor type A	Sira 07ATEX1088X	EN 60079-0:2006 EN 60079-1:2004																													
15.2																															

1	Translation												
2	EU-Type Examination Certificate												
3	Supplement 3												
4	Equipment intended for use in potentially explosive atmospheres Directive 2014/34/EU												
5	EU-Type Examination Certificate Number: BVS 15 ATEX E 064 X												
6	Product: Gas detector Type G888C Type G888S Type G999C Type G999S Type G999E Type G999P												
7	Manufacturer: GfG Gesellschaft für Gerätebau mbH												
8	Address: Klönnestr. 99, 44143 Dortmund, Germany												
9	This supplementary certificate extends EU-Type Examination Certificate No. BVS 15 ATEX E 064 X to apply to products designed and constructed in accordance with the specification set out in the appendix of the said certificate but having any acceptable variations specified in the appendix to this certificate and the documents referred to therein.												
10	DEKRA EXAM GmbH, Notified Body number 0168, in accordance with Article 17 of Directive 2014/34/EU of the European Parliament and of the Council, dated 26 February 2014, certifies that this product has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of products intended for use in potentially explosive atmospheres given in Annex II to the Directive.												
11	The examination and test results are recorded in the confidential Report No. BVS PP 15.2110 EU.												
12	Compliance with the Essential Health and Safety Requirements has been assured by compliance with: EN 60079-0:2012 + A11:2013 General requirements EN 60079-1:2014 Flameproof enclosure "d" EN 60079-11:2012 Intrinsic Safety												
13	If the sign "X" is placed after the certificate number, it indicates that the product is subject to the Special Conditions for Use specified in the appendix to this certificate.												
14	This EU-Type Examination Certificate relates only to the design and construction of the specified product. Further requirements of the Directive apply to the manufacturing process and supply of this product. These are not covered by this certificate.												
15	The marking of the product shall include the following:												
16	<table border="1"> <tr> <td>II 2G Ex ia db IIC T4 Gb</td> <td>for type G888C, G999C, G999S</td> </tr> <tr> <td>I M2 Ex ia db I Mb</td> <td>for type G888S</td> </tr> <tr> <td>II 2G Ex ia db IIC T4 Gb</td> <td>for type G888S</td> </tr> <tr> <td>I M1 Ex ia I Ma</td> <td>for type G999E, G999P</td> </tr> <tr> <td>II 1G Ex ia IIC T4 Ga</td> <td>for type G999E, G999P</td> </tr> <tr> <td>I M1 Ex ia I Ma</td> <td>for type G999E, G999P</td> </tr> </table>	II 2G Ex ia db IIC T4 Gb	for type G888C, G999C, G999S	I M2 Ex ia db I Mb	for type G888S	II 2G Ex ia db IIC T4 Gb	for type G888S	I M1 Ex ia I Ma	for type G999E, G999P	II 1G Ex ia IIC T4 Ga	for type G999E, G999P	I M1 Ex ia I Ma	for type G999E, G999P
II 2G Ex ia db IIC T4 Gb	for type G888C, G999C, G999S												
I M2 Ex ia db I Mb	for type G888S												
II 2G Ex ia db IIC T4 Gb	for type G888S												
I M1 Ex ia I Ma	for type G999E, G999P												
II 1G Ex ia IIC T4 Ga	for type G999E, G999P												
I M1 Ex ia I Ma	for type G999E, G999P												
17	DEKRA EXAM GmbH Bochum, 2018-01-02												
18	Signed: Jörg Koch Certifier												
19	Signed: Dr. Franz Eickhoff Approver												
20	<p>Page 1 of 3 of BVS 15 ATEX E 064 X / N3</p> <p>This certificate may only be reproduced in its entirety and without any change.</p> <p>DEKRA EXAM GmbH, Dinnendahlstrasse 9, 44609 Bochum, Germany. Telephone +49 234 3595-105, fax +49 234 3595-110, zs-exam@dekra.com</p>												

